

# Technical Information

## Liquisys M CCM223/253

Measurement of free chlorine/chlorine dioxide/  
total chlorine

### Transmitter for chlorine sensors



#### Application

- Drinking water
- Water treatment
- Cooling water
- Gas scrubbers
- Reverse osmosis
- Food processing
- Swimming pool water

#### Your benefits

- Field or panel-mounted housing
- Universal application
- pH compensation for free chlorine
- Simple handling
  - Logically arranged menu structure
  - Calibration via CAL button
- Safe operation
  - Overvoltage (lightning) protection
  - Manual contact control and user-defined alarm configuration

The basic unit can be extended with:

- 2 or 4 additional contacts for use as:
  - Limit contacts (also for temperature)
  - P(ID) controller for chlorine and pH
  - Timer for simple rinse processes
  - Complete cleaning with Chemoclean
- Plus package:
  - Manual pH compensation for Cl<sub>2</sub>
  - Any current output configuration via table
  - Automatic cleaning start
  - Process monitoring and live check of sensor
- HART or PROFIBUS PA / DP
- 2nd current output for temperature, main measured value or actuating variable
- Current input for flow rate monitoring with controller shut off or for feedforward control

## Function and system design

<b>Features of the basic version (EK)</b>	<p><b>Measurement of free chlorine, chlorine dioxide and total chlorine</b></p> <p>The sensor is selected from the menu. The <b>temperature</b> is displayed but the reading can also be hidden. The EP version has an alternative feature that allows simultaneous display of the pH and redox measurements.</p> <p><b>Calibration</b></p> <p>The CCS140/141 sensors for free chlorine and the CCS240/241 sensors for chlorine dioxide are zero-current-free and therefore require only <b>single-point calibration</b>. This is carried out by entering a DPD reference measured value.</p> <p>The sensor CCS120 is also calibrated by entering a DPD reference measured value. Additionally you can calibrate the zero point of the sensor CCS120 (recommended for measurements below 0.1 mg/l).</p> <p><b>Configuration</b></p> <p>Different alarms are required depending on application and operator. Therefore the transmitter permits independent <b>configuration of the alarm contact and error current</b> for each individual error. Unnecessary or undesirable alarms can be suppressed in this manner. <b>Up to four contacts Up to two contacts</b> can be used as limit contacts (also for temperature), to implement a P(ID) controller or for cleaning functions.</p> <p>Direct <b>manual operation of the contacts</b> (bypassing the menu) provides quick access to limit, control or cleaning contacts, permitting speedy correction of deviations.</p> <p>The <b>serial numbers</b> of the instrument and modules and the order code can be called up on the display.</p>
<b>Additional functions of the Plus package (ES)</b>	<p><b>Current output configuration</b></p> <p>In order to output wide measuring ranges while still achieving a high resolution in specific ranges, the <b>current output</b> can be configured as required via a table. This permits <b>bilinear</b> or <b>quasi-logarithmic</b> curves, etc.</p> <p><b>Manual pH compensation for free chlorine</b></p> <p>Measurement of free chlorine with amperometric sensors is pH-dependent while DPD measurement used for calibration is pH-independent. <b>Manual pH compensation</b> means the instrument can also be used to measure a variable pH value with a slow rate of change.</p> <p><b>Process Check System (PCS)</b></p> <p>It comprises two independent safety functions:</p> <ul style="list-style-type: none"> <li>▪ Errors in applications <b>without</b> control are detected by monitoring the limit between plausible and implausible measured values, i.e. <b>the alarm threshold</b>.</li> <li>▪ Errors in applications <b>with</b> control are detected by the <b>controller monitor</b> which monitors freely adjustable, maximum permissible time intervals and reference value overshoot or undershoot.</li> </ul> <p><b>Live check</b></p> <p>The live check issues an alarm when the sensor signal does not change over a defined period of time. This may be caused by blocking, passivation, separation from the process, etc.</p>
<b>Additional functions of version EP</b>	<p><b>Alternatively measurement of pH or ORP</b></p> <p>This extension allows additional measurement of pH value or ORP in an instrument. It also allows control of the pH value in the process.</p> <p>Automatic pH compensation means the instrument can also be used to measure a variable pH value which is subject to frequent changes.</p>
<b>Second current output</b>	<p>The second current output is freely configurable for the output of temperature, of the main measured value (free chlorine, chlorine dioxide, total chlorine) or actuating variable.</p>
<b>Current input</b>	<p>The current input of the transmitter allows two different applications: controller shut-down in case of lower flow rate violation or total failure in the main flow as well as feedforward control. Both functions are also combinable.</p>

**Measuring system**

A complete measuring system comprises:

**Version 1** (free chlorine and chlorine dioxide)

- The transmitter Liquisys M CCM223 or CCM253
- A membrane covered sensor CCS140/141 for Cl<sub>2</sub> or CCS240/241 for ClO<sub>2</sub> or an open sensor 963 for Cl<sub>2</sub>
- A flow assembly CCA250 (not necessary for sensor 963)

and optional:


- A pH or ORP sensor
- An INS proximity switch for flow monitoring (omitted with 963 sensor)
- CMK extension cable for chlorine measurement if required
- CYK71 extension cable for pH/ORP measurement if required
- MK extension cable for INS proximity switch if required
- VBC junction box

**Version 2** (total chlorine)

- The transmitter Liquisys M CCM223 or CCM253
- A sensor for total chlorine CCS120
- A flow assembly CCA250 or immersion assembly CYA611
- A special measuring cable CPK9, PM wire internally

and optional:


- A pH or ORP sensor
- An INS proximity switch for flow monitoring (omitted with immersion assembly)
- CMK extension cable (PM wire internally) for chlorine measurement if required
- CYK71 extension cable for pH/ORP measurement if required
- MK extension cable for INS proximity switch if required
- VBC junction box

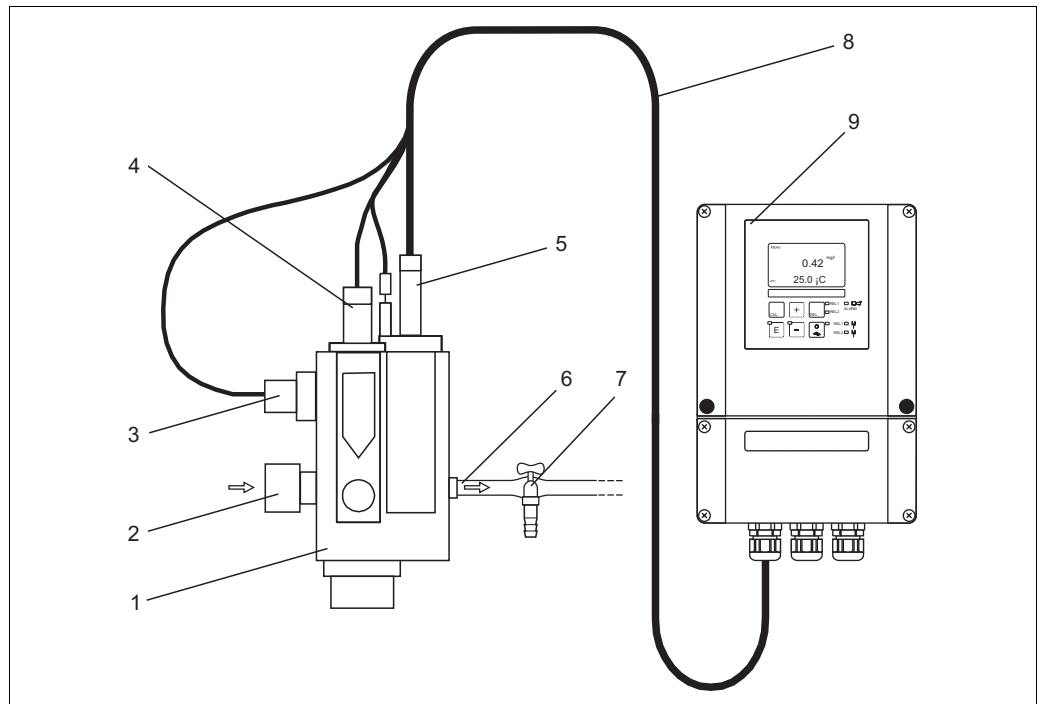

Measuring system with flow assembly (example)

- |   |                                      |   |                 |
|---|--------------------------------------|---|-----------------|
| 1 | Flow assembly CCA250                 | 6 | Medium outlet   |
| 2 | Medium inlet                         | 7 | Sampling tap    |
| 3 | Proximity switch for flow monitoring | 8 | Measuring cable |
| 4 | Mounting place for pH/redox sensor   | 9 | Transmitter     |
| 5 | Chlorine sensor                      |   |                 |

a0001691

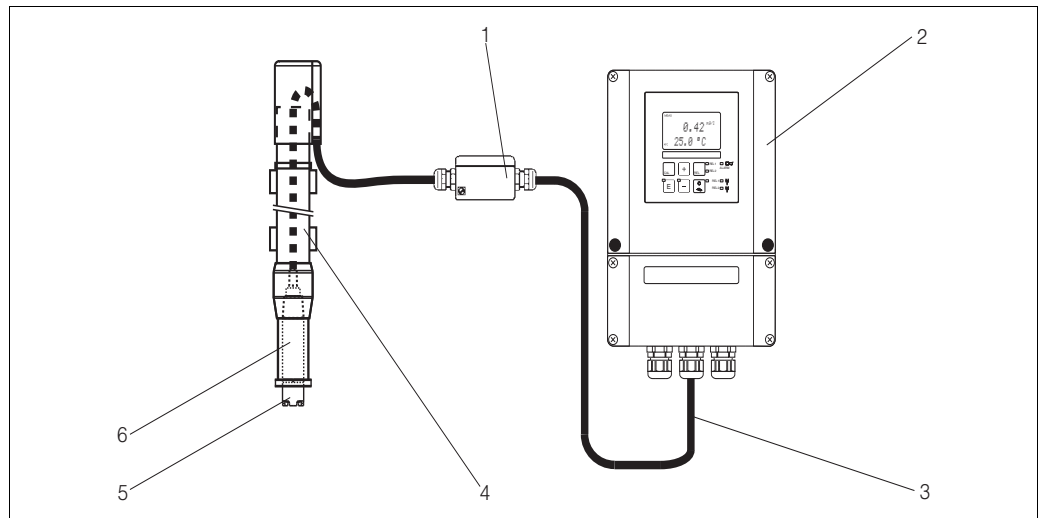

a0001791

Measuring system with immersion assembly (example)

1 Junction box

2 Transmitter

3 Measuring cable

4 Immersion assembly CYA611

5 Chlorine sensor CCS120

6 Assembly adapter G1

## Input

<b>Measured variables</b>	Total chlorine, free chlorine, chlorine dioxide, temperature pH or ORP (optional)	
<b>Cl<sub>2</sub>/ClO<sub>2</sub> measurement</b>	Display and measuring range	0 to 5 / 0 to 20 mg/l
	Application measuring range	
	CCS120	0.1 to 10 mg/l
	CCS140/240	0.05 to 20 mg/l
	CCS141/241	0.01 to 5 mg/l
	963	0.05 to 5 mg/l
	Temperature compensation range	
	CCS140/240/141/241 and 963	2 to 45 °C (36 to 113 °F)
	CCS120	5 to 45 °C (41 to 113 °F)
	pH compensation range	pH 4 to 9
	for free chlorine	
	Calibration range	pH 4 to 8
	Reference point	25 °C (77 °F) / pH 7.2
	for nominal slope	
<b>Cable specification</b>	Chlorine/chlorine dioxide sensors	max. 30 m (98 ft) with CMK cable
	CCS140/141/240/241:	
	Chlorine sensor 963:	max. 30 m (98 ft) with MK cable
	Total chlorine sensor CCS120:	max. 15 m (49 ft) with CPK9 cable
	pH/ORP measurement:	max. 50 m (164 ft) with CYK71 cable
<b>Cl<sub>2</sub>/ClO<sub>2</sub> signal input</b>	CCS120/140/141/240/241:	0 to 5000 nA
	Sensor 963:	-100 to 500 µA
<b>Temperature measurement</b>	Temperature sensor with	NTC, 10 kΩ at 25 °C (77 °F)
	CCS120/140/141/240/241:	
	Display range	0 to 50 °C (32 to 122 °F)
<b>pH and ORP measurement</b>	pH measuring range:	pH 3.5 to 9.5
	ORP measuring range:	0 to 1500 mV
	Zero point adjustment:	±100 mV
	Slope adjustment:	38 to 65 mV/pH
<b>Binary inputs</b>	Voltage:	10 ... 50 V
	Power consumption:	max. 10 mA
<b>Current input</b>	4 to 20 mA, galvanically separated	
	Load: 260 Ω at 20 mA (voltage drop 5.2 V)	

## Output

**Output signal** 0/4 to 20 mA, galvanically separated, active

HART	
Signal coding	Frequency Shift Keying (FSK) + 0.5 mA via current output signal
Data transfer rate	1200 Baud
Galvanic isolation	yes

PROFIBUS PA	
Signal coding	Manchester Bus Powered (MBP)
Data transfer rate	31.25 kBit/s, voltage mode
Galvanic isolation	yes (IO-Module)

PROFIBUS DP	
Signal coding	RS485
Data transfer rate	9.6 kBd, 19.2 kBd, 93.75 kBd, 187.5 kBd, 500 kBd, 1.5 MBd
Galvanic isolation	yes (IO-Module)

**Signal on alarm** 2.4 or 22 mA in case of an error

**Load** maximum 500  $\Omega$

**Transmission range**

Cl <sub>2</sub> /ClO <sub>2</sub> :	0 to 10 mg/l for CCS120 0 to 20 mg/l for CCS140/240 0 to 5 mg/l for CCS141/241 and 963
Temperature:	0 to 50 °C (32 to 122 °F)
pH:	pH 4 to 9
ORP:	0 to 1500 mV

**Resolution** max. 700 digits/mA

**Isolation voltage** max. 350 V<sub>RMS</sub>/500 V DC

**Overvoltage protection** according to EN 61000-4-5

**Auxiliary voltage output**

Output voltage:	15 V ± 0.6
Output current:	max. 10 mA

**Contact outputs**

Switching current with ohmic load (cos $\varphi$ = 1):	max. 2 A
Switching current with inductive load (cos $\varphi$ = 0.4):	max. 2 A
Switching voltage:	max. 250 V AC, 30 V DC
Switching power with ohmic load (cos $\varphi$ = 1):	max. 500 VA AC, 60 W DC
Switching power with inductive load (cos $\varphi$ = 0.4):	max. 500 VA AC, 60 W DC

**Limit contactor** Pickup/dropout delay: 0 to 2000 s

<b>Controller</b>	Function (adjustable):	Pulse-length/pulse-frequency controller, three-point step controller for Cl <sub>2</sub> /ClO <sub>2</sub>
	Controller response:	P, PI, PD, PID, basic load dosing
	Controller gain K <sub>p</sub> :	0.01 to 20.00
	Integral action time T <sub>n</sub> :	0.0 to 999.9 min
	Derivative action time T <sub>v</sub> :	0.0 to 999.9 min
	Period length of pulse-length controller:	0.5 to 999.9 s
	Frequency for pulse-frequency controller:	60 to 180 min <sup>-1</sup>
	Basic load:	0 to 40% of max. set value
	Motor run time for three-point step controller:	10 to 999 s
	Neutral zone for three-point step controller:	0 to 40 %

---

<b>Alarm</b>	Function (switchable):	Latching/momentary contact
	Alarm threshold adjustment range:	Cl <sub>2</sub> /ClO <sub>2</sub> /pH/ORP/temperature: total measuring range
	Alarm delay:	0 to 2000 s (min)
	Monitoring time lower limit violation:	0 to 2000 min
	Monitoring time upper limit violation:	0 to 2000 min

## Protocol specific data

<b>HART</b>	
Manufacturer ID	11 <sub>h</sub>
Device type code	0096 <sub>h</sub>
Transmitter specific revision	0002 <sub>h</sub>
HART specification	5.0
DD files	<a href="http://www.products.endress.com/hart">www.products.endress.com/hart</a>
Load HART	250 Ω
Device variables	None (dynamic variables PV, SV, only)
Features supported	-

<b>PROFIBUS PA</b>	
Manufacturer ID	11 <sub>h</sub>
Ident number	1519 <sub>h</sub>
Device revision	11 <sub>h</sub>
Profile version	2.0
GSD files	<a href="http://www.products.endress.com/profibus">www.products.endress.com/profibus</a>
GSD file version	
Output values	Main value, temperature value
Input values	Display value of PLC
Features supported	Device locking: The device can be locked by hardware or software.


<b>PROFIBUS DP</b>	
Manufacturer ID	11 <sub>h</sub>
Ident number	151D <sub>h</sub>
Profile version	2.0
GSD files	<a href="http://www.products.endress.com/profibus">www.products.endress.com/profibus</a>
GSD file version	
Output values	Main value, temperature value
Input values	Display value of PLC
Features supported	Device locking: The device can be locked by hardware or software.



## Power supply

### Electrical connection variant 1

The wiring diagram shows the connections of the transmitter with all options

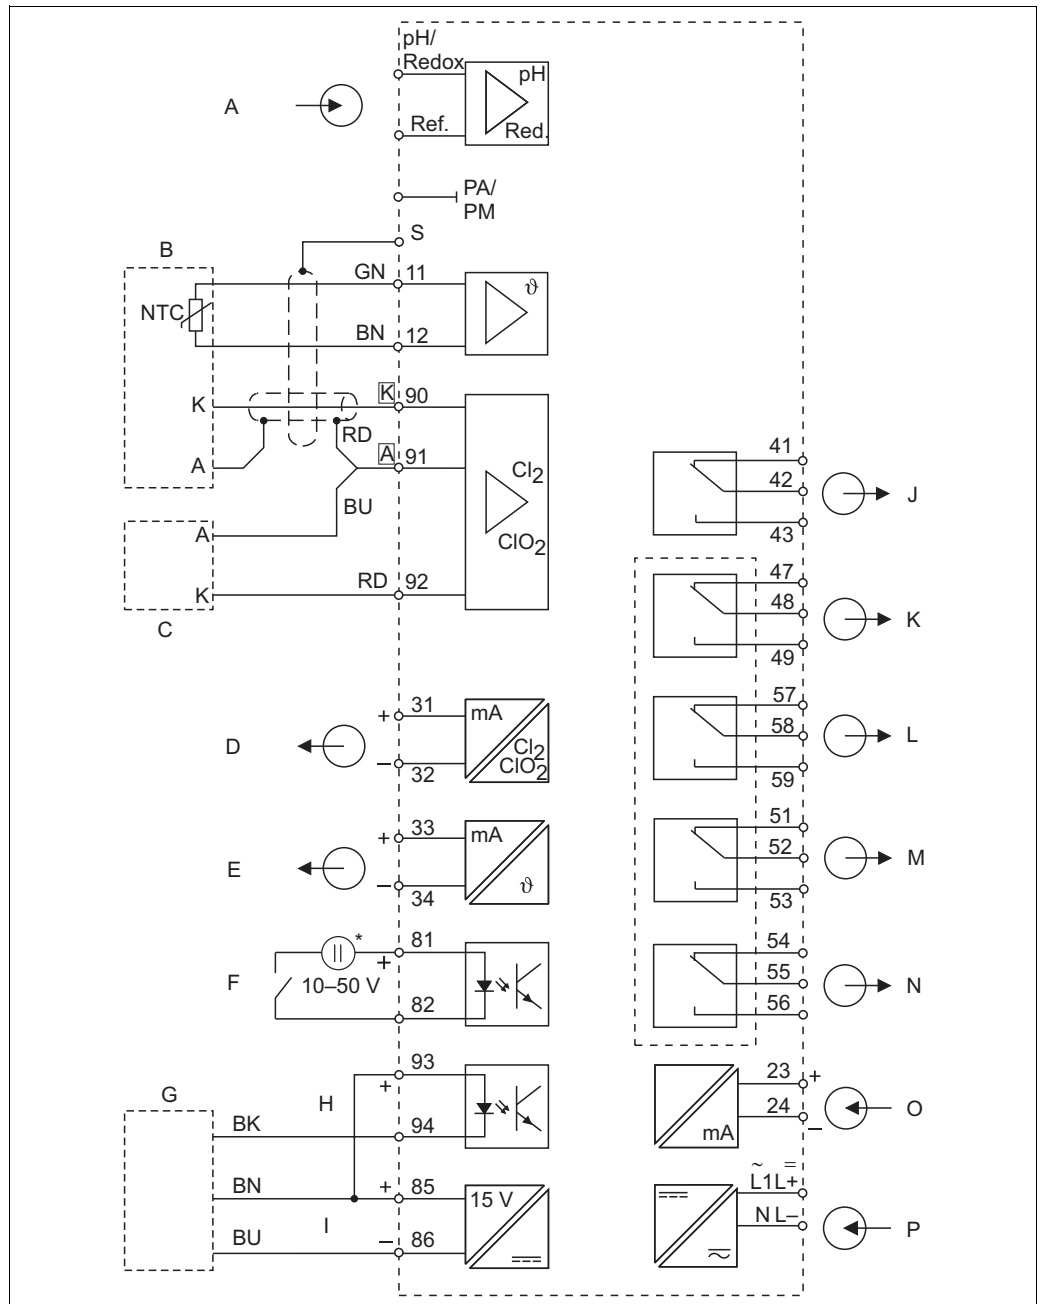

a0001903

Electrical connection of the transmitter (version 1)

A	pH / ORP input (optional)	I	Aux. voltage output
B	Sensor CCS140/141/240/241	J	Alarm (current-free contact position)
C	Sensor 963 (alternative)	K	Relay 1 (current-free contact position)
D	Signal output 1 chlorine / chlorine dioxide	L	Relay 2 (current-free contact position)
E	Signal output 2 temperature, pH or ORP	M	Relay 3 (current-free contact position)
F	Binary input 1 (hold / cleaning)	N	Relay 4 (current-free contact position)
G	Proximity switch INS	O	Current input 4 to 20 mA
H	Binary input 2	P	Power supply
*	Aux. voltage output terminal 85/86 applicable		




The device is approved for protection class II and is generally operated without protective ground connection.

The circuits "E" and "I" are not galvanically separated from each other.

## Electrical connection variant 2 (total chlorine)

The wiring diagram shows the connections of the transmitter with all options

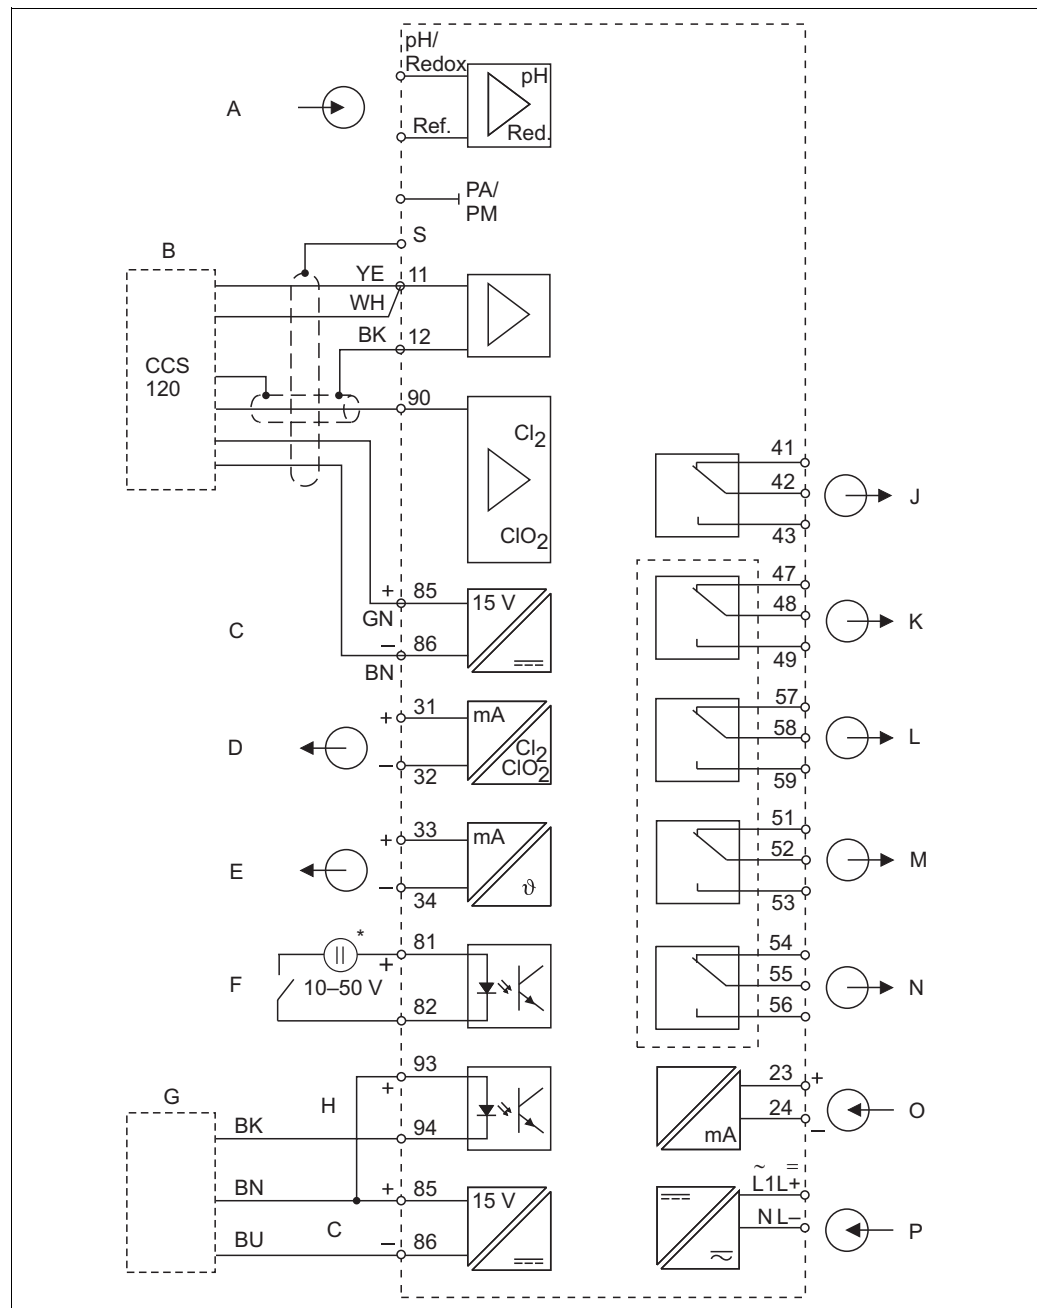

a0001904

### Electrical connection of the transmitter (version 2)

A	pH / ORP input (optional)	J	Alarm (current-free contact position)
B	Sensor CCS120	K	Relay 1 (current-free contact position)
C	Aux. voltage output	L	Relay 2 (current-free contact position)
D	Signal output 1 total chlorine	M	Relay 3 (current-free contact position)
E	Signal output 2 temperature, pH or ORP	N	Relay 4 (current-free contact position)
F	Binary input 1 (hold / cleaning)	O	Current input 4 to 20 mA
G	Proximity switch INS	P	Power supply
H	Binary input 2		
*	Aux. voltage output terminal 85/86 applicable		



The device is approved for protection class II and is generally operated without protective ground connection.

The circuits "E" and "C" are not galvanically separated from each other.

**Sensor connection**

Type of sensor	Cable	Extension
Chlorine / chlorine dioxide sensors CCS140 / 141 / 240 / 241	3 m (9.8 ft) CMK, fixed cable	VBC junction box + CMK
Chlorine sensor 963	–	VBC junction box + MK
Temperature sensor for sensor 963	CPK1	
Total chlorine sensor CCS120	CPK9-N*A1B	VBC junction box + CYK71
pH or ORP sensor without temperature sensor	CPK1 for sensors with GSA plug-in head CPK9 for sensors with ESA plug-in head	VBC junction box + CYK71

**Supply voltage**

Depending on ordered version:  
100/115/230 V AC +10/-15 %, 48 to 62 Hz  
24 V AC/DC +20/-15 %

**Fieldbus connection**

HART	
Supply voltage	n/a, active current outputs
Integrated reverse voltage protection	n/a, active current outputs

PROFIBUS PA	
Supply voltage	9 V to 32 V, max. 35 V
Polarity sensitive	no
FISCO/FNICO compliant acc. to IEC 60079-27	no

PROFIBUS DP	
Supply voltage	9 V to 32 V, max. 35 V
Polarity sensitive	n/a
FISCO/FNICO compliant acc. to IEC 60079-27	no

**Power consumption**

max. 7.5 VA

**Mains protection**

Fine-wire fuse, medium-slow blow 250 V/3.15 A

**Circuit breaker****NOTICE****The device does not have a power switch**


- ▶ You must provide a protected circuit breaker in the vicinity of the device.
- ▶ This must be a switch or a power-circuit breaker and you must label it as the circuit breaker for the device.
- ▶ At the supply point, the power supply for the 24 V versions must be isolated from dangerous live cables by double or reinforced insulation.

## Performance characteristics

<b>Cl<sub>2</sub>/ClO<sub>2</sub> measurement</b>	Measured value resolution	
	CCS120/140/240 and 963:	0.01 mg/l
	CCS141/241:	0.001 mg/l
	Measurement deviation <sup>1</sup> display (pH, T = const.)	max. 0.5 % of measured value ±4 digits
	CCS140/141/240/241:	max. 1 % of measured value ±4 digits
	CCS120 and 963:	
Repeatability:	max. 0.2 % of measuring range	
Measurement deviation <sup>1</sup> of signal output	max. 0.75 % of current output range	
<b>Temperature measurement</b>	Measured value resolution:	0.1 °C
	Measurement deviation <sup>1</sup> of display:	±0.3 K
	Measurement deviation <sup>1</sup> signal output:	max. 1.25 % of current output range
<b>pH and ORP measurement</b>	pH measured value resolution:	pH 0.01
	ORP measured value resolution:	1 mV
	Measurement deviation <sup>1</sup> of display pH:	pH 0.03
	Measurement deviation <sup>1</sup> of display ORP:	3 mV
	Measurement deviation <sup>1</sup> of pH signal output:	max. 1.25 % of current output range
	Measurement deviation <sup>1</sup> of ORP signal output:	max. 1.25 % of current output range
1) acc. to IEC 60746-1, at nominal operating conditions		


# Installation

## Installation instructions

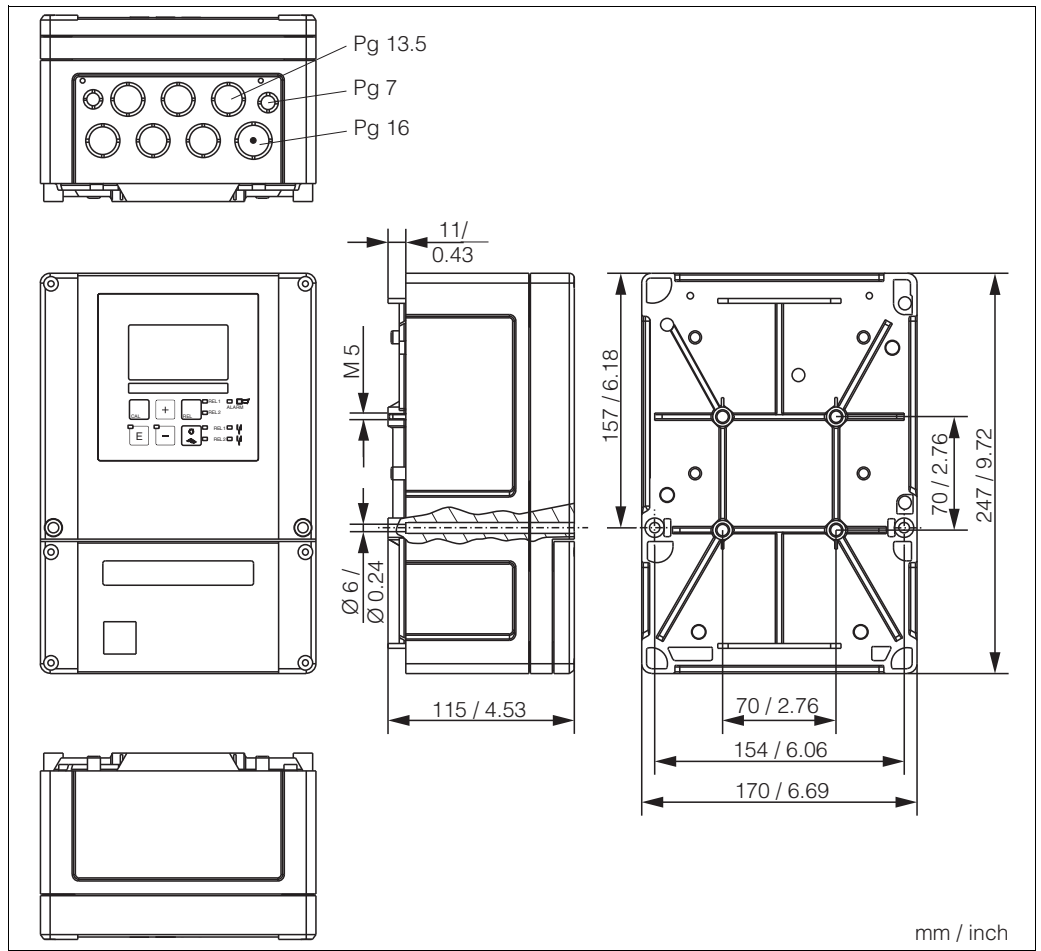


C07-CxM253xx-06-06-00-en-001.EPS

Field instrument

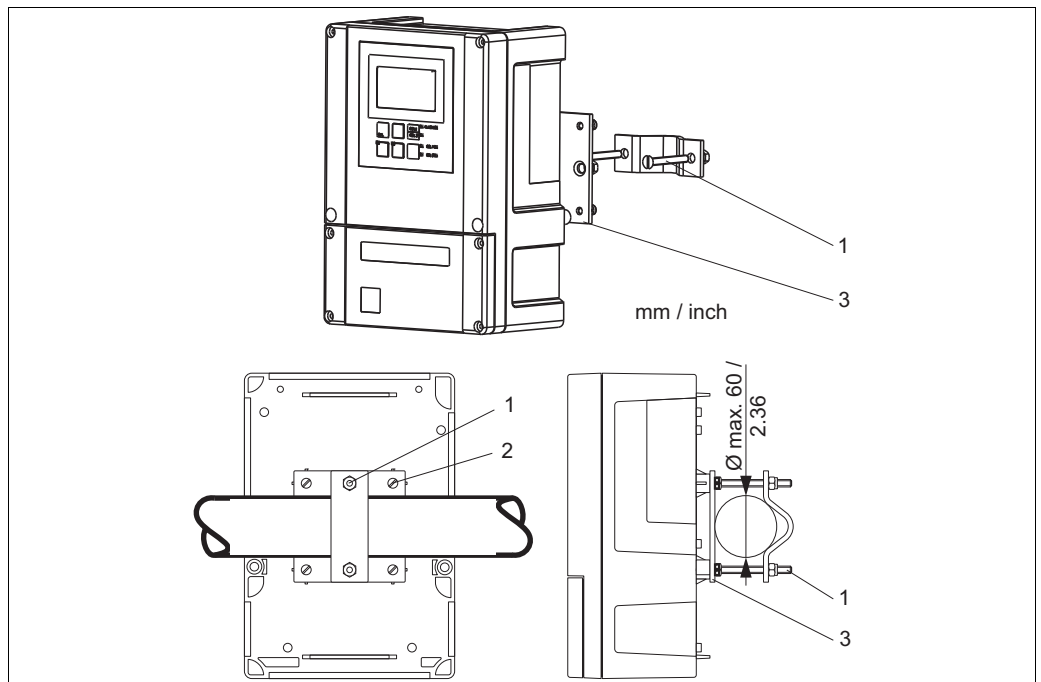

a0005737


Mounting on pipes

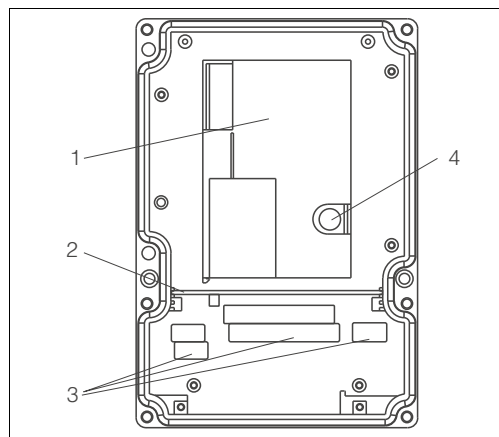

- 1 Removable electronics box
- 2 Partition plate
- 3 Terminal blocks
- 4 Fuse

C07-CxM253xx-11-06-00-xx-001.EPS


Inside of field instrument

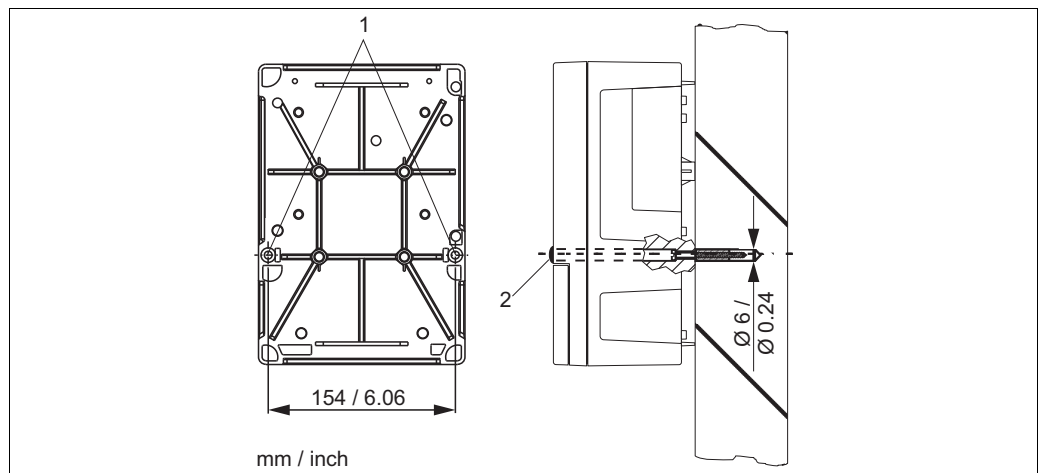

a0005736

Wall mounting of the field instrument


- 1 Mounting holes
- 2 Protecting cap

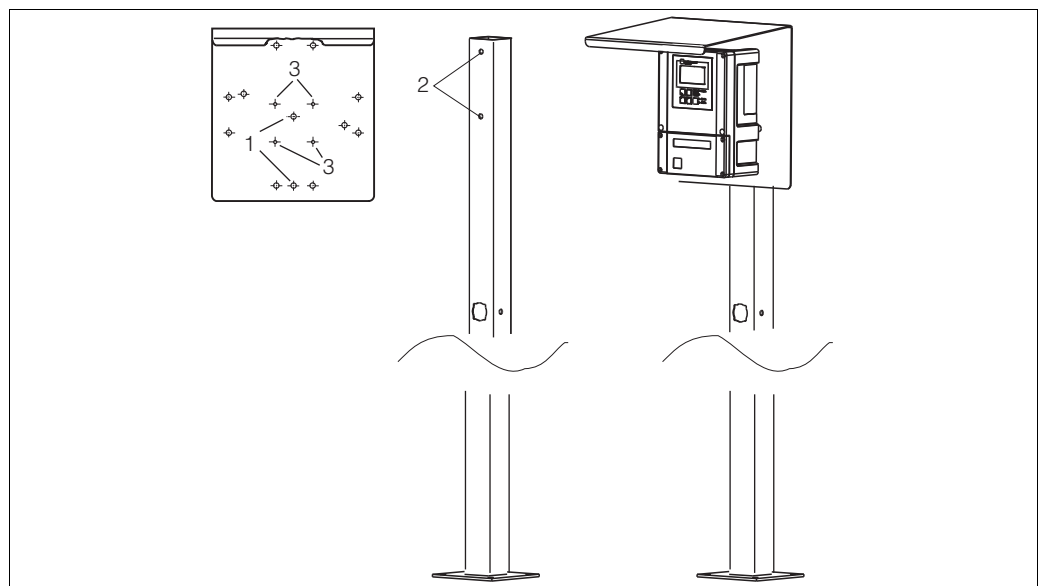


C07-CxM253xx-11-06-00-xx-004.EPS

Mounting of the field instrument with mounting post and weather protection cover

- 1-3 Mounting holes

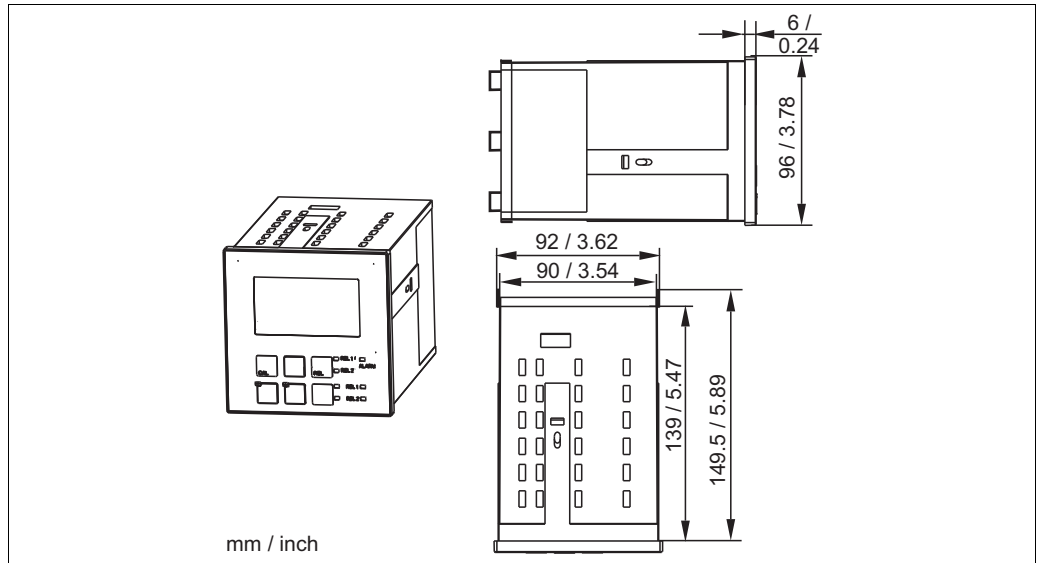

Dimensions panel-mounted instrument

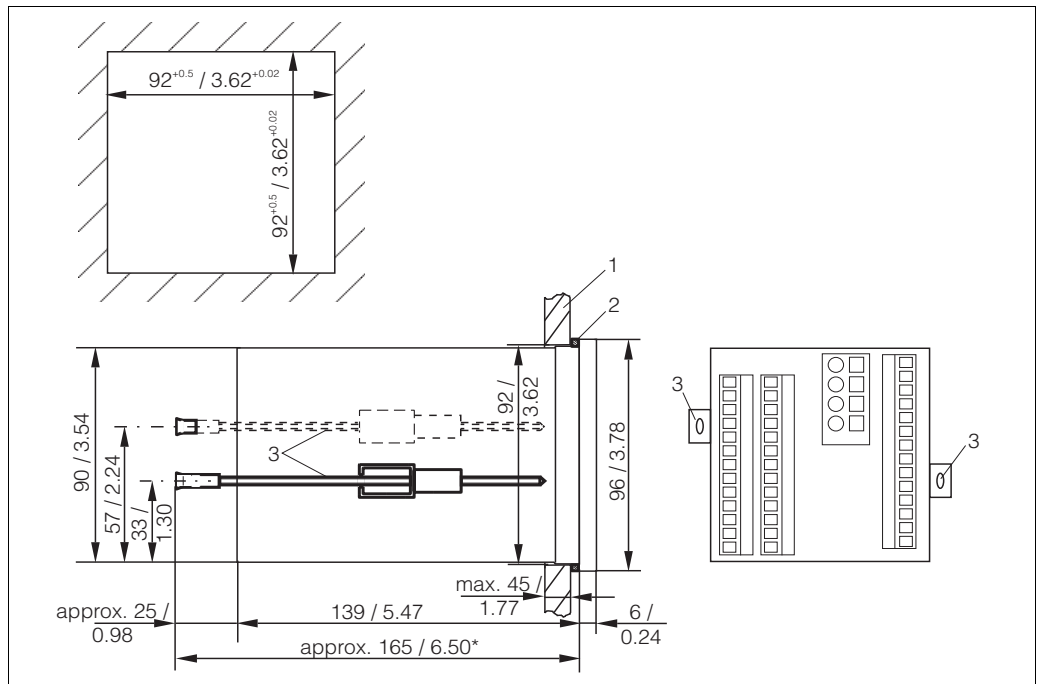

Installation of the panel-mounted instrument

- 1 Wall of control cabinet
- 2 Gasket
- 3 Tensioning screws
- \* Required installation depth

C07-CxM223xx-11-06-00-en-001.EPS

## Environment

<b>Ambient temperature</b>	-10 to +55 °C (+14 to +131 °F)	
<b>Storage temperature</b>	-25 to +65 °C (-13 to +149 °F)	
<b>Electromagnetic compatibility</b>	Interference emission and interference immunity as per EN 61326-1:2006, EN 61326-2-3:2006	
<b>Ingress protection</b>	Panel mounted instrument: Field instrument:	IP 54 (front), IP 30 (housing) IP 65 / tightness acc. to NEMA 4X
<b>Electrical safety</b>	according EN/IEC 61010-1:2001, Installation Category II, for use up to 2000 m above sea level	
<b>CSA</b>	Apparatus with CSA General Purpose Approval are certified for indoor use.	
<b>Relative humidity</b>	10 to 95%, non-condensing	
<b>Pollution degree</b>	The product is suitable for pollution degree 2.	

## Mechanical construction

<b>Dimensions</b>	Panel-mounted instrument: Field instrument:	96 x 96 x 145 mm (3.78 x 3.78 x 5.71 inches) Installation depth: approx. 165 mm (6.50") 247 x 170 x 115 mm (9.72 x 6.69 x 4.53 inches)
<b>Weight</b>	Panel-mounted instrument: Field instrument:	max. 0.7 kg (1.5 lb) max. 2.3 kg (5.1 lb)
<b>Material</b>	Housing of panel-mounted instrument: Field housing: Front membrane:	Polycarbonate ABS PC Fr Polyester, UV-resistant
<b>Terminals</b>	Cross section	max. 2.5 mm <sup>2</sup> (14 AWG)




## Operability

### Operating concept

All instrument control functions are arranged in a logical menu structure. Following access code entry, the individual parameters can be easily selected and modified as needed.

### Display elements

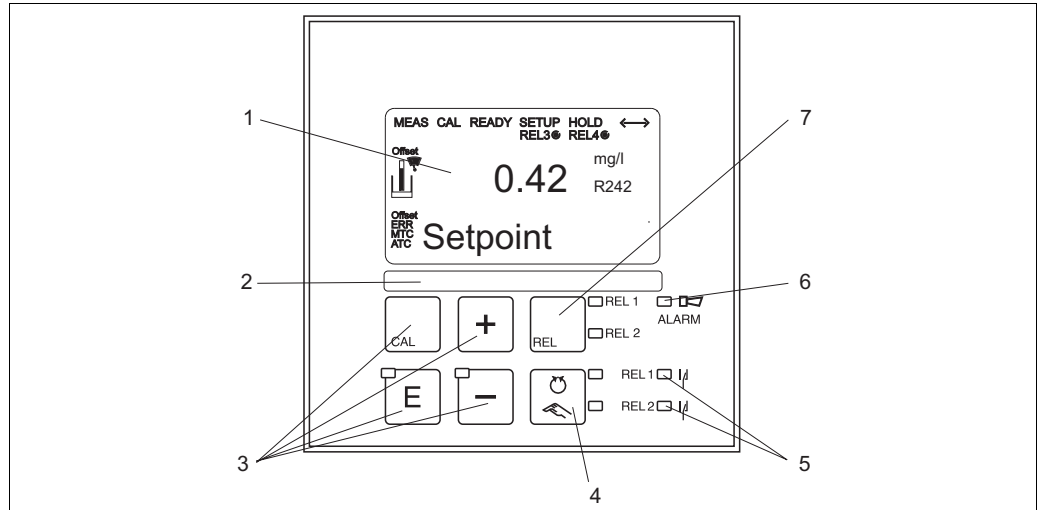

#### Operating elements

- 1 LC display for displaying the measured values and configuration data
- 2 Field for user labelling
- 3 4 main operating keys for calibration and device configuration
- 4 Changeover switch for automatic/manual mode of the relays
- 5 LEDs for limit contactor relay (switch status)
- 6 LED for alarm function
- 7 Display of the active contact and key for relay changeover in manual mode

## Certificates and approvals

### CE symbol

#### Declaration of conformity

The product meets the legal requirements of the harmonized European standards. The manufacturer confirms compliance with the standards by affixing the CE symbol.

### CSA General Purpose

#### CSA General Purpose

The products listed below are eligible to bear the CSA Mark shown with adjacent indicators "C" and "US":

Version	Approval
CCM253-..2... CCM253-..3... CCM253-..7...	CSA Mark for Canada and USA
CCM223-..2... CCM223-..3... CCM223-..7...	CSA Mark for Canada and USA

## Ordering information

### Order code

Enter the following address into your browser to access the relevant product page:  
[www.products.endress.com/ccm223](http://www.products.endress.com/ccm223) or  
[www.products.endress.com/ccm253](http://www.products.endress.com/ccm253)

1. You can choose from the following options on the product page located on the right:

Product page function
:: Add to product list
:: Price & order information
:: Compare this product
:: Configure this product

2. Click "Configure this product".
3. The configurator opens in a separate window. You can now configure your device and receive the complete order code that applies for the device.
4. Afterwards, export the order code as a PDF or Excel file. To do so, click the appropriate button at the top of the page.

### Product structure

Input, software version	
EK	Chlorine/chlorine dioxide/total chlorine measurement, basic version
ES	Chlorine/chlorine dioxide/total chlorine measurement, with additional functions (Plus package)
EP	Chlorine/chlorine dioxide/total chlorine measurement, with additional functions (Plus package) with additional pH or ORP measurement (switchable)
Power supply; approval	
0	230 V AC
1	115 V AC
2	230 V AC; CSA Gen. Purp.
3	115 V AC; CSA Gen. Purp.
5	100 V AC
7	24 V AC/DC; CSA Gen. Purp.
8	24 V AC/DC
Output	
0	1 x 20 mA, primary value
1	2 x 20 mA, primary value + secondary value
3	PROFIBUS PA
4	PROFIBUS DP
5	1 x 20 mA, primary value, HART
6	2 x 20 mA, primary value, HART + secondary value
Additional contacts	
05	not selected
10	2 relays (limit/P(ID)/timer)
15	4 relays (limit/P(ID)/Chemoclean) <b>(not with PROFIBUS DP)</b>
16	4 relays (limit/P(ID)/timer) <b>(not with PROFIBUS DP)</b>
20	1 x 4 to 20 mA input + 2 relays (limit/P(ID)/timer)
25	1 x 4 to 20 mA input + 4 relays (limit/P(ID)/Chemoclean) <b>(not with PROFIBUS DP)</b>
26	1 x 4 to 20 mA input + 4 relays (limit/P(ID)/timer) <b>(not with PROFIBUS DP)</b>
Marking	
1	Tagging (Tag), see additional spec.
CCM253-	complete order code
CCM223-	

**Additional functions of the Plus package****Version ES**

Compared to the basic EK version, this version is extended by the Plus package:

- Manual pH compensation for free chlorine, fields B2 and B3
- Current output table, fields O33x
- Sensor and process monitoring, function group P
- Automatic start of cleaning function, field F8.

**Version EP**

This version includes the functions of the ES version and in addition:

- Optional pH or ORP measurement, field B1
- Automatic pH compensation for free chlorine
- Sensor and process monitoring even for pH or ORP, fields P12x
- Limit contact for pH or ORP, fields R22x
- pH value control, fields R25x.

---

**Scope of delivery**

The delivery of the field instrument includes:

- 1 transmitter CCM253
- 1 plug-in screw terminal
- 1 cable gland Pg 7
- 1 cable gland Pg 16 reduced
- 2 cable glands Pg 13.5
- 1 Operating Instructions BA00214C/07/EN
- 1 Operating Instructions
  - versions with HART communication:
    - 1 Operating Instructions Field Communication with HART, BA00208C/07/EN
  - versions with PROFIBUS communication:
    - 1 Operating Instructions Field Communication with PROFIBUS PA/DP, BA00209C/07/EN

The delivery of the panel-mounted instrument includes:

- 1 transmitter CCM223
- 1 set of plug-in screw terminals
- 2 tensioning screws
- 1 Operating Instructions
- 1 Operating Instructions BA00214C/07/EN
- versions with HART communication:
  - 1 Operating Instructions Field Communication with HART, BA00208C/07/EN
- versions with PROFIBUS communication:
  - 1 Operating Instructions Field Communication with PROFIBUS PA/DP, BA00209C/07/EN

## Accessories

### Sensors

#### CCS120

- Amperometric sensor for total chlorine
- Measuring range 0.1 to 10 mg/l
- Ordering acc. to product structure, [www.products.endress.com/ccs120](http://www.products.endress.com/ccs120)
- Technical Information TI00388C/07/EN

#### CCS140

- Membrane-covered amperometric sensor for free chlorine
- Measuring range 0.05 to 20 mg/l
- Ordering acc. to product structure, [www.products.endress.com/ccs140](http://www.products.endress.com/ccs140)
- Technical Information TI00058C/07/EN

#### CCS141

- Membrane-covered amperometric trace sensor for free chlorine
- Measuring range 0.01 to 5 mg/l
- Ordering acc. to product structure, [www.products.endress.com/ccs141](http://www.products.endress.com/ccs141)
- Technical Information TI00058C/07/EN

#### CCS240

- Membrane-covered amperometric sensor for chlorine dioxide
- Measuring range 0.05 to 20 mg/l
- Ordering acc. to product structure, [www.products.endress.com/ccs240](http://www.products.endress.com/ccs240)
- Technical Information (TI00114C/07/EN)

#### CCS241

- Membrane-covered amperometric trace sensor for chlorine dioxide
- Measuring range 0.01 to 5 mg/l
- Ordering acc. to product structure, [www.products.endress.com/ccs241](http://www.products.endress.com/ccs241)
- Technical Information (TI00114C/07/EN)

### Connection accessories

#### CYK71 measuring cable

- Non-terminated cable for the connection of sensors or the extension of sensor cables
- Sold by the meter, order numbers:
  - non-Ex version, black: 50085333
  - Ex version, blue: 51506616

#### CMK measuring cable

- For cable extension between junction box and transmitter, non terminated, sold by the meter
- Order no. 50005374

#### CPK1 measuring cable

- For pH/ORP electrodes with GSA plug-in head
- Ordering acc. to product structure, see Technical Information (TI00118C/07/EN)

#### Measuring cable CPK9-N\*A1B internal PM wire

- For sensors with TOP68 plug-in head, for high-temperature and high-pressure applications, IP 68
- Ordering acc. to product structure, see Technical Information (TI 00118C/07/EN)

#### MK extension cable

- Two-wire signal cable with additional screen and PVC insulation.
- Particularly for the transmission of output signals of transmitters or input signals of controllers and for temperature measurement.
- Order no. 50000662

#### Junction box VBC

- Metallic junction box for cable extension,
- Dimensions (W x D x H): 125 x 80 x 54 mm / 4.92 x 3.15 x 2.13 inches
- Order no. 50005181


Junction box VBM

- For cable extension
- 10 terminals
- Cable entries: 2 x Pg 13.5 or 2 x NPT ½"
- Material: aluminum
- Ingress protection: IP 65 (≅ NEMA 4X)
- Order numbers:
  - cable entries Pg 13.5: 50003987
  - cable entries NPT ½": 51500177

**Mounting accessories**

CYY101 weather protection cover for field devices, absolutely essential if operating the unit outdoors


- Material: stainless steel 1.4031 (AISI 304)
- Order No. CYY101-A

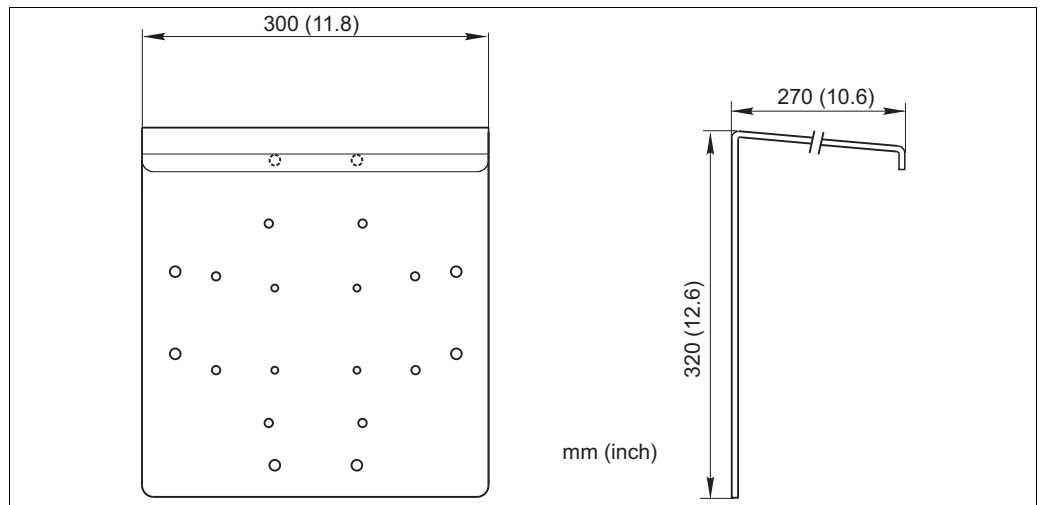

Weather protection cover for field devices

## Post mounting kit


- For mounting of field housing on horizontal or vertical pipes ( $\varnothing$  max. 60 mm (2.36"))
- Material: stainless steel 1.4301
- order no. 50086842

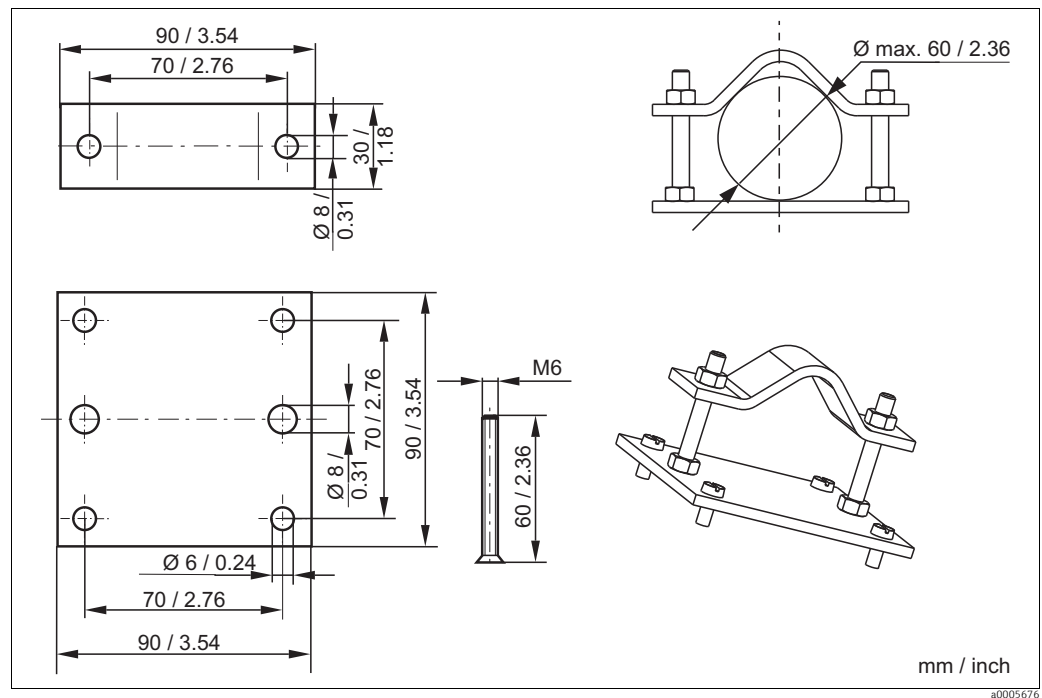

Post mounting kit

## CYY102 universal post

- Square pipe for mounting transmitters
- Material: stainless steel 1.4301 (AISI 304)
- Order No. CYY102-A

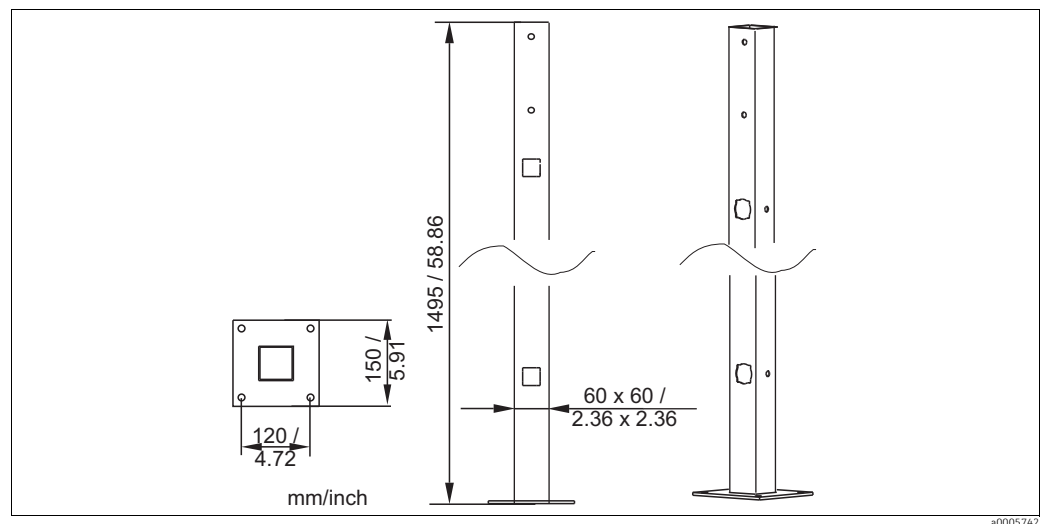

Universal post

**Measuring system**

Compact measuring station CCE10/CCE11

- Panel mounted ready for connection for holding one transmitter, with flow assembly CCA250
  - Ordering acc. to product structure, s. Technical Information TI00440C/07/EN
- 

**Calibration tool**

CCM182

- Microprocessor-controlled photometer for determining chlorine and pH value
- Measuring range for chlorine: 0.05 to 6 mg/l
- Measuring range for pH value: 6.5 to 8.4
- Order no.: CCM182-0

[www.addresses.endress.com](http://www.addresses.endress.com)

---