

# Technical Information

## Proline Promass I 100

Coriolis flowmeter



Combines in-line viscosity and flow measurement with an ultra-compact transmitter

### Application

- Measuring principle operates independently of physical fluid properties such as viscosity or density
- Measuring liquids and gases in applications requiring low pressure loss and gentle fluid treatment

### Device properties

- Straight, easy cleanable single-tube system
- TMB® technology
- Measuring tube made of Titanium
- Robust, ultra-compact transmitter housing
- High ingress protection: IP69K
- Local display available

### Your benefits

- Energy-saving – minimum pressure loss thanks to full-bore design
- Fewer process measuring points – multivariable measurement (flow, density, temperature)
- Space-saving installation – no in/outlet run needs
- Space-saving transmitter – full functionality on smallest footprint
- Time-saving local operation without additional software and hardware – integrated web server
- Integrated verification – Heartbeat Technology™

## Table of contents







<b>Document information</b> . . . . .	<b>4</b>	Shock resistance . . . . .	44
Symbols used . . . . .	4	Vibration resistance . . . . .	44
<b>Function and system design</b> . . . . .	<b>5</b>	Interior cleaning . . . . .	44
Measuring principle . . . . .	5	Electromagnetic compatibility (EMC) . . . . .	45
Measuring system . . . . .	6	<b>Process</b> . . . . .	<b>45</b>
Device architecture . . . . .	7	Medium temperature range . . . . .	45
Safety . . . . .	7	Density . . . . .	45
<b>Input</b> . . . . .	<b>7</b>	Pressure-temperature ratings . . . . .	45
Measured variable . . . . .	7	Secondary containment pressure rating . . . . .	48
Measuring range . . . . .	8	Flow limit . . . . .	48
Operable flow range . . . . .	9	Pressure loss . . . . .	49
<b>Output</b> . . . . .	<b>9</b>	System pressure . . . . .	49
Output signal . . . . .	9	Thermal insulation . . . . .	49
Signal on alarm . . . . .	10	Heating . . . . .	50
Ex connection data . . . . .	12	Vibrations . . . . .	51
Low flow cut off . . . . .	13	<b>Mechanical construction</b> . . . . .	<b>52</b>
Galvanic isolation . . . . .	13	Design, dimensions . . . . .	52
Protocol-specific data . . . . .	13	Weight . . . . .	71
<b>Power supply</b> . . . . .	<b>19</b>	Materials . . . . .	72
Terminal assignment . . . . .	19	Process connections . . . . .	74
Pin assignment, device plug . . . . .	25	<b>Operability</b> . . . . .	<b>74</b>
Supply voltage . . . . .	27	Operating concept . . . . .	74
Power consumption . . . . .	27	Local display . . . . .	74
Current consumption . . . . .	28	Remote operation . . . . .	74
Power supply failure . . . . .	28	Service interface . . . . .	76
Electrical connection . . . . .	28	<b>Certificates and approvals</b> . . . . .	<b>78</b>
Potential equalization . . . . .	32	CE mark . . . . .	78
Terminals . . . . .	32	C-Tick symbol . . . . .	78
Cable entries . . . . .	33	Ex approval . . . . .	78
Cable specification . . . . .	33	Hygienic compatibility . . . . .	79
<b>Performance characteristics</b> . . . . .	<b>34</b>	Certification PROFIBUS . . . . .	79
Reference operating conditions . . . . .	34	Modbus RS485 certification . . . . .	79
Maximum measured error . . . . .	34	EtherNet/IP certification . . . . .	79
Repeatability . . . . .	36	Pressure Equipment Directive . . . . .	79
Response time . . . . .	36	Other standards and guidelines . . . . .	79
Influence of ambient temperature . . . . .	36	<b>Ordering information</b> . . . . .	<b>80</b>
Influence of medium temperature . . . . .	36	<b>Application packages</b> . . . . .	<b>80</b>
Influence of medium pressure . . . . .	37	Heartbeat Technology . . . . .	80
Design fundamentals . . . . .	37	Concentration . . . . .	81
<b>Installation</b> . . . . .	<b>38</b>	Viscosity . . . . .	81
Mounting location . . . . .	38	<b>Accessories</b> . . . . .	<b>81</b>
Orientation . . . . .	40	Device-specific accessories . . . . .	81
Inlet and outlet runs . . . . .	40	Communication-specific accessories . . . . .	81
Special mounting instructions . . . . .	40	Service-specific accessories . . . . .	82
Mounting Safety Barrier Promass 100 . . . . .	42	System components . . . . .	83
<b>Environment</b> . . . . .	<b>42</b>	<b>Documentation</b> . . . . .	<b>83</b>
Ambient temperature range . . . . .	42	Standard documentation . . . . .	83
Storage temperature . . . . .	44	Supplementary device-dependent documentation . . . . .	83
Climate class . . . . .	44		
Degree of protection . . . . .	44		

**Registered trademarks . . . . . 84**









## Document information

### Symbols used


#### Electrical symbols



Symbol	Meaning
	<b>Direct current</b> A terminal to which DC voltage is applied or through which direct current flows.
	<b>Alternating current</b> A terminal to which alternating voltage is applied or through which alternating current flows.
	<b>Direct current and alternating current</b> <ul style="list-style-type: none"> <li>▪ A terminal to which alternating voltage or DC voltage is applied.</li> <li>▪ A terminal through which alternating current or direct current flows.</li> </ul>
	<b>Ground connection</b> A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.
	<b>Protective ground connection</b> A terminal which must be connected to ground prior to establishing any other connections.
	<b>Equipotential connection</b> A connection that has to be connected to the plant grounding system: This may be a potential equalization line or a star grounding system depending on national or company codes of practice.

#### Symbols for certain types of information

Symbol	Meaning
	<b>Permitted</b> Indicates procedures, processes or actions that are permitted.
	<b>Preferred</b> Indicates procedures, processes or actions that are preferred.
	<b>Forbidden</b> Indicates procedures, processes or actions that are forbidden.
	<b>Tip</b> Indicates additional information.
	<b>Reference to documentation</b> Refers to the corresponding device documentation.
	<b>Reference to page</b> Refers to the corresponding page number.
	<b>Reference to graphic</b> Refers to the corresponding graphic number and page number.
	<b>Visual inspection</b>

#### Symbols in graphics

Symbol	Meaning
1, 2, 3, ...	Item numbers
1., 2., 3. ...	Series of steps
A, B, C, ...	Views
A-A, B-B, C-C, ...	Sections
	Flow direction

Symbol	Meaning
	<b>Hazardous area</b> Indicates a hazardous area.
	<b>Safe area (non-hazardous area)</b> Indicates the non-hazardous area.

## Function and system design

### Measuring principle

The measuring principle is based on the controlled generation of Coriolis forces. These forces are always present in a system when both translational and rotational movements are superimposed.

$$F_c = 2 \cdot \Delta m (v \cdot \omega)$$

$F_c$  = Coriolis force

$\Delta m$  = moving mass


$\omega$  = rotational velocity

$v$  = radial velocity in rotating or oscillating system

The amplitude of the Coriolis force depends on the moving mass  $\Delta m$ , its velocity  $v$  in the system and thus on the mass flow. Instead of a constant rotational velocity  $\omega$ , the sensor uses oscillation.

In the sensor, an oscillation is produced in the measuring tube. The Coriolis forces produced at the measuring tube cause a phase shift in the tube oscillations (see illustration):

- If there is zero flow (i.e. when the fluid stands still), the oscillation measured at points A and B has the same phase (no phase difference).
- Mass flow causes deceleration of the oscillation at the inlet of the tubes (2) and acceleration at the outlet (3).

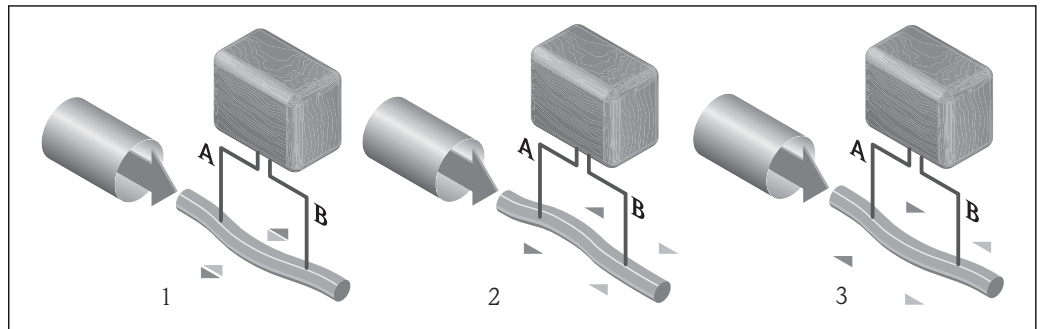

A0016772

The phase difference (A-B) increases with increasing mass flow. Electrodynamical sensors register the tube oscillations at the inlet and outlet. System balance is created by exciting an eccentrically arranged swinging mass to antiphase oscillation. The measuring principle operates independently of temperature, pressure, viscosity, conductivity and flow profile.

### Density measurement

The measuring tube is continuously excited at its resonance frequency. A change in the mass and thus the density of the oscillating system (comprising measuring tube and fluid) results in a corresponding, automatic adjustment in the oscillation frequency. Resonance frequency is thus a function of medium density. The microprocessor utilizes this relationship to obtain a density signal.

### Volume measurement

Together with the measured mass flow, this is used to calculate the volume flow.

### Temperature measurement


The temperature of the measuring tube is determined in order to calculate the compensation factor due to temperature effects. This signal corresponds to the process temperature and is also available as an output signal.

**Measuring system**


The device consists of a transmitter and a sensor. If a device with Modbus RS485 intrinsically safe is ordered, the Safety Barrier Promass 100 is part of the scope of supply and must be implemented to operate the device.

One device version is available: compact version, transmitter and sensor form a mechanical unit.


**Transmitter**
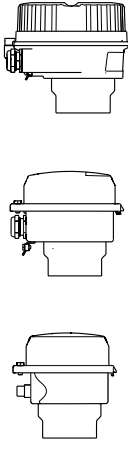
<p><b>Promass 100</b></p>  <p>A0016693</p> <p>A0016694</p> <p>A0016695</p>	<p>Device versions and materials:</p> <ul style="list-style-type: none"> <li>▪ Compact, aluminum coated: Aluminum, AlSi10Mg, coated</li> <li>▪ Compact, hygienic, stainless: Hygienic version, stainless steel 1.4301 (304)</li> <li>▪ Ultra compact, hygienic, stainless: Hygienic version, stainless steel 1.4301 (304)</li> </ul> <p>Configuration:</p> <ul style="list-style-type: none"> <li>▪ Via operating tools (e.g. FieldCare)</li> <li>▪ Additionally for device version with onsite display: Via Web browser (e.g. Microsoft Internet Explorer)</li> <li>▪ Also for device version with 4-20 mA HART, pulse/frequency/switch output: Via Web browser (e.g. Microsoft Internet Explorer)</li> <li>▪ Also for device version with EtherNet/IP output: <ul style="list-style-type: none"> <li>- Via Web browser (e.g. Microsoft Internet Explorer)</li> <li>- Via Add-on Profile Level 3 for automation system from Rockwell Automation</li> <li>- Via Electronic Data Sheet (EDS)</li> </ul> </li> </ul>
---	--


**Sensor**

<p><b>Promass I</b></p>  <p>A0016508</p>	<ul style="list-style-type: none"> <li>▪ Sensitive fluid handling thanks to straight single-tube system</li> <li>▪ Simultaneous measurement of viscosity, flow, volume flow, density and temperature (multivariable)</li> <li>▪ Immune to process influences</li> <li>▪ Nominal diameter range: DN 8 to 80 (<math>\frac{3}{8}</math> to 3")</li> <li>▪ Materials: <ul style="list-style-type: none"> <li>- Sensor: stainless steel, 1.4301/1.4307 (304L)</li> <li>- Measuring tubes: titanium Grade 9</li> <li>- Process connections: stainless steel, 1.4301 (304), wetted parts: titanium Grade 2</li> </ul> </li> </ul>
---	--

**Safety Barrier Promass 100**

 <p>A0016763</p>	<ul style="list-style-type: none"> <li>▪ Dual-channel safety barrier for installation in non-hazardous locations or Zone 2/Div. 2: <ul style="list-style-type: none"> <li>- Channel 1: DC 24 V power supply</li> <li>- Channel 2: Modbus RS485</li> </ul> </li> <li>▪ In addition to current, voltage and power limitation, it offers galvanic isolation of circuits for explosion protection.</li> <li>▪ Easy DIN rail mounting (DIN 35mm) for installation in control cabinets</li> </ul>
---	---

Device architecture

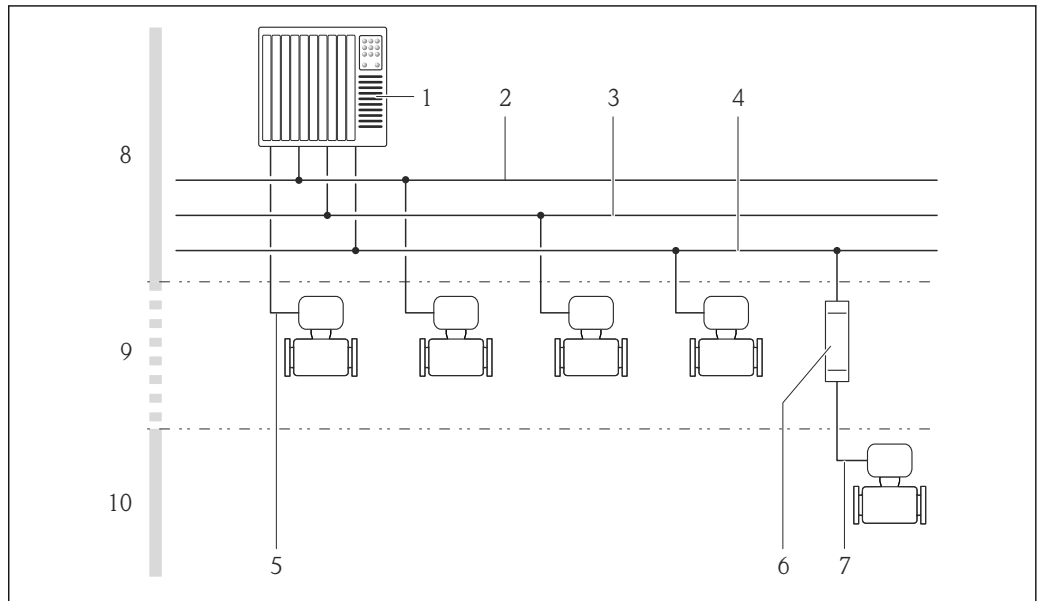

A0016779

1 Possibilities for integrating measuring devices into a system

- 1 Control system (e.g. PLC)
- 2 EtherNet/IP
- 3 PROFIBUS DP
- 4 Modbus RS485
- 5 4-20 mA HART, pulse/frequency/switch output
- 6 Safety Barrier Promass 100
- 7 Modbus RS485 intrinsically safe
- 8 Non-hazardous area
- 9 Non-hazardous area and Zone 2/Div. 2
- 10 Intrinsically safe area and Zone 1/Div. 1

Safety

IT security

We only provide a warranty if the device is installed and used as described in the Operating Instructions. The device is equipped with security mechanisms to protect it against any inadvertent changes to the device settings.

IT security measures in line with operators' security standards and designed to provide additional protection for the device and device data transfer must be implemented by the operators themselves.

Input

Measured variable

Direct measured variables

- Mass flow
- Density
- Temperature
- Viscosity

Calculated measured variables

- Volume flow
- Corrected volume flow
- Reference density

## Measuring range

## Measuring ranges for liquids

DN		Measuring range full scale values $\dot{m}_{\min(F)}$ to $\dot{m}_{\max(F)}$	
[mm]	[in]	[kg/h]	[lb/min]
8	$\frac{3}{8}$	0 to 2 000	0 to 73.50
15	$\frac{1}{2}$	0 to 6 500	0 to 238.9
15 FB	$\frac{1}{2}$ FB	0 to 18 000	0 to 661.5
25	1	0 to 18 000	0 to 661.5
25 FB	1 FB	0 to 45 000	0 to 1 654
40	$1\frac{1}{2}$	0 to 45 000	0 to 1 654
40 FB	$1\frac{1}{2}$ FB	0 to 70 000	0 to 2 573
50	2	0 to 70 000	0 to 2 573
50 FB	2 FB	0 to 180 000	0 to 6 615
80	3	0 to 180 000	0 to 6 615

FB = Full bore

## Measuring ranges for gases

The full scale values depend on the density of the gas and can be calculated with the formula below:

$$\dot{m}_{\max(G)} = \dot{m}_{\max(F)} \cdot \rho_G \cdot X$$

$\dot{m}_{\max(G)}$	Maximum full scale value for gas [kg/h]
$\dot{m}_{\max(F)}$	Maximum full scale value for liquid [kg/h]
$\dot{m}_{\max(G)} < \dot{m}_{\max(F)}$	$\dot{m}_{\max(G)}$ can never be greater than $\dot{m}_{\max(F)}$
$\rho_G$	Gas density in [kg/m <sup>3</sup> ] at operating conditions

DN		x
[mm]	[in]	[kg/m <sup>3</sup> ]
8	$\frac{3}{8}$	60
15	$\frac{1}{2}$	80
15 FB	$\frac{1}{2}$ FB	90
25	1	90
25 FB	1 FB	90
40	$1\frac{1}{2}$	90
40 FB	$1\frac{1}{2}$ FB	90
50	2	90
50 FB	2 FB	110
80	3	155 110

FB = Full bore



To calculate the measuring range, use the *Applicator* sizing tool (→ 82)

## Calculation example for gas

- Sensor: Promass I, DN 50
- Gas: Air with a density of 60.3 kg/m<sup>3</sup> (at 20 °C and 50 bar)
- Measuring range (liquid): 70 000 kg/h
- x = 90 kg/m<sup>3</sup> (for Promass I, DN 50)



Maximum possible full scale value:

$$\dot{m}_{\max(G)} = \dot{m}_{\max(F)} \cdot \rho_G : x = 70\,000 \text{ kg/h} \cdot 60.3 \text{ kg/m}^3 : 90 \text{ kg/m}^3 = 46\,900 \text{ kg/h}$$

**Recommended measuring range**

"Flow limit" section (→  48)

**Operable flow range**


Over 1000 : 1.

Flow rates above the preset full scale value are not overridden by the electronics unit, with the result that the totalizer values are registered correctly.

## Output



**Output signal**

**Current output**

<b>Current output</b>	4-20 mA HART (active)
<b>Maximum output values</b>	<ul style="list-style-type: none"> <li>▪ DC 24 V (no flow)</li> <li>▪ 22.5 mA</li> </ul>
<b>Load</b>	0 to 700 Ω
<b>Resolution</b>	0.38 µA
<b>Damping</b>	Adjustable: 0.07 to 999 s
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> <li>▪ Density</li> <li>▪ Reference density</li> <li>▪ Temperature</li> </ul> <p> The range of options increases if the measuring device has one or more application packages.</p>

**Pulse/frequency/switch output**

<b>Function</b>	Can be set to pulse, frequency or switch output
<b>Version</b>	Passive, open collector
<b>Maximum input values</b>	<ul style="list-style-type: none"> <li>▪ DC 30 V</li> <li>▪ 25 mA</li> </ul>
<b>Voltage drop</b>	For 25 mA: ≤ DC 2 V
<b>Pulse output</b>	
<b>Pulse width</b>	Adjustable: 0.05 to 2 000 ms
<b>Maximum pulse rate</b>	10 000 Impulse/s
<b>Pulse value</b>	Adjustable
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> </ul>
<b>Frequency output</b>	
<b>Output frequency</b>	Adjustable: 0 to 10 000 Hz
<b>Damping</b>	Adjustable: 0 to 999 s
<b>Pulse/pause ratio</b>	1:1

<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> <li>▪ Density</li> <li>▪ Reference density</li> <li>▪ Temperature</li> </ul> <p> The range of options increases if the measuring device has one or more application packages.</p>
<b>Switch output</b>	
<b>Switching behavior</b>	Binary, conductive or non-conductive
<b>Switching delay</b>	Adjustable: 0 to 100 s
<b>Number of switching cycles</b>	Unlimited
<b>Assignable functions</b>	<ul style="list-style-type: none"> <li>▪ Off</li> <li>▪ On</li> <li>▪ Diagnostic behavior</li> <li>▪ Limit value <ul style="list-style-type: none"> <li>- Mass flow</li> <li>- Volume flow</li> <li>- Corrected volume flow</li> <li>- Density</li> <li>- Reference density</li> <li>- Temperature</li> <li>- Totalizer 1-3</li> </ul> </li> <li>▪ Flow direction monitoring</li> <li>▪ Status <ul style="list-style-type: none"> <li>- Partially filled pipe detection</li> <li>- Low flow cut off</li> </ul> </li> </ul> <p> The range of options increases if the measuring device has one or more application packages.</p>

**PROFIBUS DP**

<b>Signal encoding</b>	NRZ code
<b>Data transfer</b>	9.6 kBaud...12 MBaud

**Modbus RS485**

<b>Physical interface</b>	In accordance with EIA/TIA-485-A standard
<b>Terminating resistor</b>	<ul style="list-style-type: none"> <li>▪ For device version used in non-hazardous areas or Zone 2/Div. 2: integrated and can be activated via DIP switches on the transmitter electronics module</li> <li>▪ For device version used in intrinsically safe areas: integrated and can be activated via DIP switches on the Safety Barrier Promass 100</li> </ul>

**EtherNet/IP**

<b>Standards</b>	In accordance with IEEE 802.3
------------------	-------------------------------

**Signal on alarm**

Depending on the interface, failure information is displayed as follows:

**Current output**

4-20 mA

<b>Failure mode</b>	Selectable (as per NAMUR recommendation NE 43): <ul style="list-style-type: none"> <li>▪ Minimum value: 3.6 mA</li> <li>▪ Maximum value: 22 mA</li> <li>▪ Defined value: 3.59 to 22.5 mA</li> <li>▪ Actual value</li> <li>▪ Last valid value</li> </ul>
---------------------	---

HART

<b>Device diagnostics</b>	Device condition can be read out via HART Command 48
---------------------------	--

**Pulse/frequency/switch output**

<b>Pulse output</b>	
<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>▪ Actual value</li> <li>▪ No pulses</li> </ul>
<b>Frequency output</b>	
<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>▪ Actual value</li> <li>▪ Defined value: 0 to 12 500 Hz</li> <li>▪ 0 Hz</li> </ul>
<b>Switch output</b>	
<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>▪ Current status</li> <li>▪ Open</li> <li>▪ Closed</li> </ul>

**PROFIBUS DP**

<b>Status and alarm messages</b>	Diagnostics in accordance with PROFIBUS PA Profile 3.02
----------------------------------	---

**Modbus RS485**

<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>▪ NaN value instead of current value</li> <li>▪ Last valid value</li> </ul>
---------------------	---

**EtherNet/IP**

<b>Device diagnostics</b>	Device condition can be read out in Input Assembly
---------------------------	--

**Local display**

<b>Plain text display</b>	With information on cause and remedial measures
<b>Backlight</b>	Red backlighting indicates a device error.

 Status signal as per NAMUR recommendation NE 107

**Operating tool**

- Via digital communication:
  - HART protocol
  - PROFIBUS DP
  - Modbus RS485
  - EtherNet/IP
- Via service interface

Plain text display	With information on cause and remedial measures
--------------------	---



Additional information on remote operation (→ 74)

**Web browser**

Plain text display	With information on cause and remedial measures
--------------------	---

**Light emitting diodes (LED)**

<b>Status information</b>	<p>Status indicated by various light emitting diodes</p> <p>The following information is displayed depending on the device version:</p> <ul style="list-style-type: none"> <li>■ Supply voltage active</li> <li>■ Data transmission active</li> <li>■ Device alarm/error has occurred</li> <li>■ EtherNet/IP network available</li> <li>■ EtherNet/IP connection established</li> </ul>
---------------------------	---

**Ex connection data**

These values only apply for the following device version:  
Order code for "Output", option **M**: Modbus RS485, for use in intrinsically safe areas

**Safety Barrier Promass 100***Safety-related values*


Terminal numbers			
Supply voltage		Signal transmission	
2 (L-)	1 (L+)	26 (A)	27 (B)
$U_{\text{nom}} = \text{DC } 24 \text{ V}$ $U_{\text{max}} = \text{AC } 260 \text{ V}$		$U_{\text{nom}} = \text{DC } 5 \text{ V}$ $U_{\text{max}} = \text{AC } 260 \text{ V}$	

*Intrinsically safe values*

Terminal numbers			
Supply voltage		Signal transmission	
20 (L-)	10 (L+)	62 (A)	72 (B)
$U_o = 16.24 \text{ V}$ $I_o = 623 \text{ mA}$ $P_o = 2.45 \text{ W}$ For IIC*: $L_o = 92.8 \mu\text{H}$ , $C_o = 0.433 \mu\text{F}$ , $L_o/R_o = 14.6 \mu\text{H}/\Omega$ For IIB*: $L_o = 372 \mu\text{H}$ , $C_o = 2.57 \mu\text{F}$ , $L_o/R_o = 58.3 \mu\text{H}/\Omega$			
* The gas group depends on the sensor and nominal diameter.			
For an overview and for information on the interdependencies between the gas group - sensor - nominal diameter, see the "Safety Instructions" (XA) document for the measuring device			

**Transmitter**

*Intrinsically safe values*

Order code for "Approvals"	Terminal numbers			
	Supply voltage		Signal transmission	
	20 (L-)	10 (L+)	62 (A)	72 (B)
<ul style="list-style-type: none"> <li>▪ Option <b>BM</b>: ATEX II2G + IECEx Z1 Ex ia, II2D Ex tb</li> <li>▪ Option <b>BO</b>: ATEX II1/2G + IECEx Z0/Z1 Ex ia, II2D</li> <li>▪ Option <b>BQ</b>: ATEX II1/2G + IECEx Z0/Z1 Ex ia</li> <li>▪ Option <b>BU</b>: ATEX II2G + IECEx Z1 Ex ia</li> <li>▪ Option <b>C2</b>: CSA C/US IS Cl. I, II, III Div. 1</li> <li>▪ Option <b>85</b>: ATEX II2G + IECEx Z1 Ex ia + CSA C/US IS Cl. I, II, III Div. 1</li> </ul>	$U_i = 16.24 \text{ V}$ $I_i = 623 \text{ mA}$ $P_i = 2.45 \text{ W}$ $L_i = 0 \text{ } \mu\text{H}$ $C_i = 6 \text{ nF}$			
 For an overview and for information on the interdependencies between the gas group - sensor - nominal diameter, see the "Safety Instructions" (XA) document for the measuring device				


**Low flow cut off** The switch points for low flow cut off are user-selectable.

**Galvanic isolation** The following connections are galvanically isolated from each other:

- Outputs
- Power supply

**Protocol-specific data** **HART**

<b>Manufacturer ID</b>	0x11
<b>Device type ID</b>	0x4A
<b>HART protocol revision</b>	7.0
<b>Device description files (DTM, DD)</b>	Information and files under: <a href="http://www.endress.com">www.endress.com</a>
<b>HART load</b>	Min. 250 $\Omega$

<b>Dynamic variables</b>	<p>Read out the dynamic variables: HART command 3 The measured variables can be freely assigned to the dynamic variables.</p> <p><b>Measured variables for PV (primary dynamic variable)</b></p> <ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> <li>▪ Density</li> <li>▪ Reference density</li> <li>▪ Temperature</li> </ul> <p><b>Measured variables for SV, TV, QV (secondary, tertiary and quaternary dynamic variable)</b></p> <ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> <li>▪ Density</li> <li>▪ Reference density</li> <li>▪ Temperature</li> <li>▪ Totalizer 1</li> <li>▪ Totalizer 2</li> <li>▪ Totalizer 3</li> </ul> <p> The range of options increases if the measuring device has one or more application packages.</p> <p><b>Heartbeat Technology Application Package</b> Additional measured variables are available with the Heartbeat Technology application package:</p> <ul style="list-style-type: none"> <li>▪ Sensor integrity</li> <li>▪ Carrier pipe temperature</li> <li>▪ Frequency fluctuation 1</li> <li>▪ Oscillation amplitude 1</li> <li>▪ Tube damping fluctuation 1</li> <li>▪ Exciter current 1</li> </ul>
<b>Device variables</b>	<p>Read out the device variables: HART command 9 The device variables are permanently assigned.</p> <p>A maximum of 8 device variables can be transmitted:</p> <ul style="list-style-type: none"> <li>▪ 0 = mass flow</li> <li>▪ 1 = volume flow</li> <li>▪ 2 = corrected volume flow</li> <li>▪ 3 = density</li> <li>▪ 4 = reference density</li> <li>▪ 5 = temperature</li> <li>▪ 6 = totalizer 1</li> <li>▪ 7 = totalizer 2</li> <li>▪ 8 = totalizer 3</li> <li>▪ 9 = dynamic viscosity</li> <li>▪ 10 = kinematic viscosity</li> <li>▪ 11 = temp. compensated dynamic viscosity</li> <li>▪ 12 = temp. compensated kinematic viscosity</li> <li>▪ 13 = target mass flow</li> <li>▪ 14 = carrier mass flow</li> <li>▪ 15 = concentration</li> </ul>


### PROFIBUS DP

<b>Manufacturer ID</b>	0x11
<b>Ident number</b>	0x1561
<b>Profile version</b>	3.02
<b>Device description files (GSD, DTM, DD)</b>	Information and files under: <ul style="list-style-type: none"> <li>▪ <a href="http://www.endress.com">www.endress.com</a></li> <li>▪ <a href="http://www.profibus.org">www.profibus.org</a></li> </ul>

<p><b>Output values</b> (from measuring device to automation system)</p>	<p><b>Analog input 1 to 8</b></p> <ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> <li>▪ Target mass flow</li> <li>▪ Carrier mass flow</li> <li>▪ Density</li> <li>▪ Reference density</li> <li>▪ Concentration</li> <li>▪ Dynamic viscosity</li> <li>▪ Kinematic viscosity</li> <li>▪ Temp. compensated dynamic viscosity</li> <li>▪ Temp. compensated kinematic viscosity</li> <li>▪ Temperature</li> <li>▪ Carrier pipe temperature</li> <li>▪ Electronic temperature</li> <li>▪ Oscillation frequency</li> <li>▪ Oscillation amplitude</li> <li>▪ Frequency fluctuation</li> <li>▪ Oscillation damping</li> <li>▪ Tube damping fluctuation</li> <li>▪ Signal asymmetry</li> <li>▪ Exciter current</li> </ul> <p><b>Digital input 1 to 2</b></p> <ul style="list-style-type: none"> <li>▪ Partially filled pipe detection</li> <li>▪ Low flow cut off</li> </ul> <p><b>Totalizer 1 to 3</b></p> <ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> </ul>
<p><b>Input values</b> (from automation system to measuring device)</p>	<p><b>Analog output 1 to 3 (fixed assignment)</b></p> <ul style="list-style-type: none"> <li>▪ Pressure</li> <li>▪ Temperature</li> <li>▪ Reference density</li> </ul> <p><b>Digital output 1 to 3 (fixed assignment)</b></p> <ul style="list-style-type: none"> <li>▪ Digital output 1: switch positive zero return on/off</li> <li>▪ Digital output 2: perform zero point adjustment</li> <li>▪ Digital output 3: switch switch output on/off</li> </ul> <p><b>Totalizer 1 to 3</b></p> <ul style="list-style-type: none"> <li>▪ Totalize</li> <li>▪ Reset and hold</li> <li>▪ Preset and hold</li> <li>▪ Stop</li> <li>▪ Operating mode configuration: <ul style="list-style-type: none"> <li>- Net flow total</li> <li>- Forward flow total</li> <li>- Reverse flow total</li> </ul> </li> </ul>
<p><b>Supported functions</b></p>	<ul style="list-style-type: none"> <li>▪ Identification &amp; Maintenance Simplest device identification on the part of the control system and nameplate</li> <li>▪ PROFIBUS upload/download Reading and writing parameters is up to ten times faster with PROFIBUS upload/download</li> <li>▪ Condensed status Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur</li> </ul>
<p><b>Configuration of the device address</b></p>	<ul style="list-style-type: none"> <li>▪ DIP switches on the I/O electronics module</li> <li>▪ Via operating tools (e.g. FieldCare)</li> </ul>

**Modbus RS485**

Protocol	Modbus Applications Protocol Specification V1.1
Device type	Slave
Slave address range	1 to 247


Broadcast address range	0
Function codes	<ul style="list-style-type: none"> <li>▪ 03: Read holding register</li> <li>▪ 04: Read input register</li> <li>▪ 06: Write single registers</li> <li>▪ 08: Diagnostics</li> <li>▪ 16: Write multiple registers</li> <li>▪ 23: Read/write multiple registers</li> </ul>
Broadcast messages	Supported by the following function codes: <ul style="list-style-type: none"> <li>▪ 06: Write single registers</li> <li>▪ 16: Write multiple registers</li> <li>▪ 23: Read/write multiple registers</li> </ul>
Supported baud rate	<ul style="list-style-type: none"> <li>▪ 1 200 BAUD</li> <li>▪ 2 400 BAUD</li> <li>▪ 4 800 BAUD</li> <li>▪ 9 600 BAUD</li> <li>▪ 19 200 BAUD</li> <li>▪ 38 400 BAUD</li> <li>▪ 57 600 BAUD</li> <li>▪ 115 200 BAUD</li> </ul>
Data transfer mode	<ul style="list-style-type: none"> <li>▪ ASCII</li> <li>▪ RTU</li> </ul>
Data access	Each device parameter can be accessed via Modbus RS485.  For Modbus register information (-> 83)

### EtherNet/IP

Protocol	<ul style="list-style-type: none"> <li>▪ The CIP Networks Library Volume 1: Common Industrial Protocol</li> <li>▪ The CIP Networks Library Volume 2: EtherNet/IP Adaptation of CIP</li> </ul>
Communication type	<ul style="list-style-type: none"> <li>▪ 10Base-T</li> <li>▪ 100Base-TX</li> </ul>
Device profile	Generic device (product type: 0x2B)
Manufacturer ID	0x49E
Device type ID	0x104A
Baud rates	Automatic <sup>10</sup> / <sub>100</sub> Mbit with half-duplex and full-duplex detection
Polarity	Auto-polarity for automatic correction of crossed TxD and RxD pairs
Supported CIP connections	Max. 3 connections
Explicit connections	Max. 6 connections
I/O connections	Max. 6 connections (scanner)
Configuration options for measuring device	<ul style="list-style-type: none"> <li>▪ DIP switches on the electronics module for IP addressing</li> <li>▪ Manufacturer-specific software (FieldCare)</li> <li>▪ Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>▪ Web browser</li> <li>▪ Electronic Data Sheet (EDS) integrated in the measuring device</li> </ul>
Configuration of the EtherNet interface	<ul style="list-style-type: none"> <li>▪ Speed: 10 MBit, 100 MBit, auto (factory setting)</li> <li>▪ Duplex: half-duplex, full-duplex, auto (factory setting)</li> </ul>
Configuration of the device address	<ul style="list-style-type: none"> <li>▪ DIP switches on the electronics module for IP addressing (last octet)</li> <li>▪ DHCP</li> <li>▪ Manufacturer-specific software (FieldCare)</li> <li>▪ Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>▪ Web browser</li> <li>▪ EtherNet/IP tools, e.g. RSLinx (Rockwell Automation)</li> </ul>
Device Level Ring (DLR)	No




Fix Input			
RPI	5 ms to 10 s (factory setting: 20 ms)		
Exclusive Owner Multicast		Instance	Size [byte]
	Instance configuration:	0x68	398
	O → T configuration:	0x66	64
	T → O configuration:	0x64	44
Exclusive Owner Multicast		Instance	Size [byte]
	Instance configuration:	0x69	-
	O → T configuration:	0x66	64
	T → O configuration:	0x64	44
Input only Multicast		Instance	Size [byte]
	Instance configuration:	0x68	398
	O → T configuration:	0xC7	-
	T → O configuration:	0x64	44
Input only Multicast		Instance	Size [byte]
	Instance configuration:	0x69	-
	O → T configuration:	0xC7	-
	T → O configuration:	0x64	44
Input Assembly	<ul style="list-style-type: none"> <li>■ Current device diagnostics</li> <li>■ Mass flow</li> <li>■ Volume flow</li> <li>■ Corrected volume flow</li> <li>■ Density</li> <li>■ Reference density</li> <li>■ Temperature</li> <li>■ Totalizer 1</li> <li>■ Totalizer 2</li> <li>■ Totalizer 3</li> </ul>		
Configurable Input			
RPI	5 ms to 10 s (factory setting: 20 ms)		
Exclusive Owner Multicast		Instance	Size [byte]
	Instance configuration:	0x68	398
	O → T configuration:	0x66	64
	T → O configuration:	0x65	88
Exclusive Owner Multicast		Instance	Size [byte]
	Instance configuration:	0x69	-
	O → T configuration:	0x66	64
	T → O configuration:	0x65	88
Input only Multicast		Instance	Size [byte]
	Instance configuration:	0x68	398
	O → T configuration:	0xC7	-
	T → O configuration:	0x65	88
Input only Multicast		Instance	Size [byte]
	Instance configuration:	0x69	-
	O → T configuration:	0xC7	-
	T → O configuration:	0x65	88

Configurable Input Assembly	<ul style="list-style-type: none"> <li>▪ Current device diagnostics</li> <li>▪ Mass flow</li> <li>▪ Volume flow</li> <li>▪ Corrected volume flow</li> <li>▪ Density</li> <li>▪ Reference density</li> <li>▪ Temperature</li> <li>▪ Totalizer 1</li> <li>▪ Totalizer 2</li> <li>▪ Totalizer 3</li> </ul> <p> The range of options increases if the measuring device has one or more application packages.</p>
Fix Output	
Output Assembly	<ul style="list-style-type: none"> <li>▪ Activation of reset totalizers 1-3</li> <li>▪ Activation of pressure compensation</li> <li>▪ Activation of reference density compensation</li> <li>▪ Activation of temperature compensation</li> <li>▪ Reset totalizers 1-3</li> <li>▪ External pressure value</li> <li>▪ Pressure unit</li> <li>▪ External reference density</li> <li>▪ Reference density unit</li> <li>▪ External temperature</li> <li>▪ Temperature unit</li> </ul>
Configuration	
Configuration Assembly	<p>Only the most common configurations are listed below.</p> <ul style="list-style-type: none"> <li>▪ Software write protection</li> <li>▪ Mass flow unit</li> <li>▪ Mass unit</li> <li>▪ Volume flow unit</li> <li>▪ Volume unit</li> <li>▪ Corrected volume flow unit</li> <li>▪ Corrected volume unit</li> <li>▪ Density unit</li> <li>▪ Reference density unit</li> <li>▪ Temperature unit</li> <li>▪ Pressure unit</li> <li>▪ Length</li> <li>▪ Totalizer 1-3: <ul style="list-style-type: none"> <li>- Assignment</li> <li>- Unit</li> <li>- Measuring mode</li> <li>- Failure mode</li> </ul> </li> <li>▪ Alarm delay</li> </ul>

# Power supply

Terminal assignment

Overview: housing version

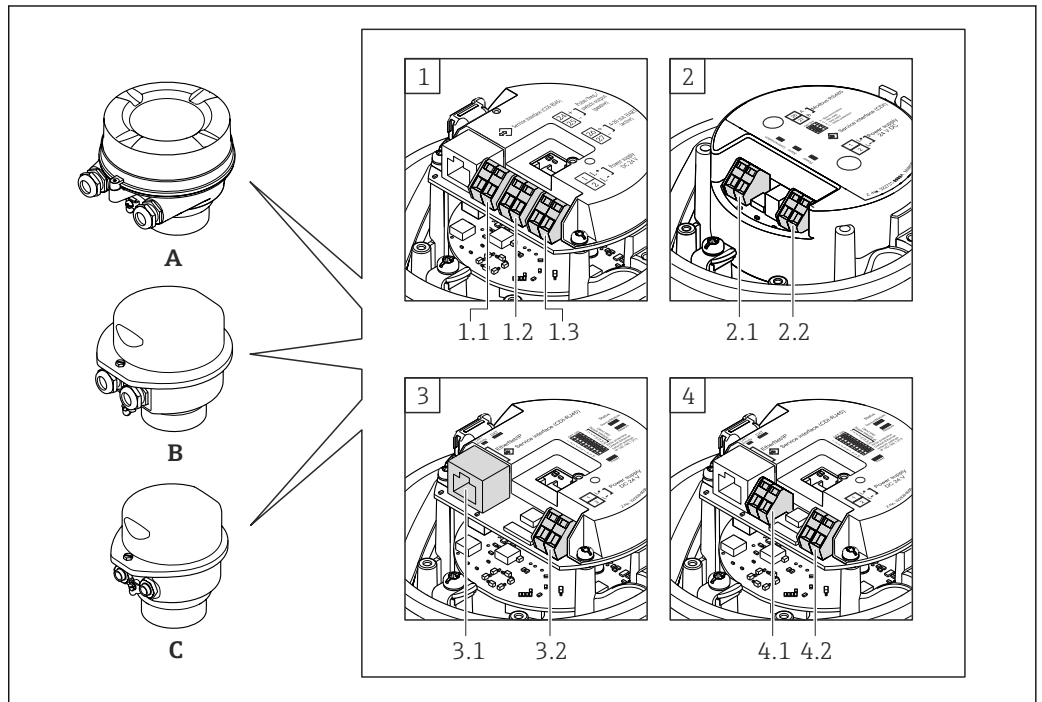

A0016770

- A Housing version: compact, aluminum coated
- B Housing version: compact, hygienic, stainless
- C Housing version: ultra compact, hygienic, stainless, M12 device plug
- 1 Connection version: 4-20 mA HART, pulse/frequency/switch output
  - 1.1 Signal transmission: pulse/frequency/switch output
  - 1.2 Signal transmission: 4-20 mA HART
  - 1.3 Supply voltage
- 2 Connection version: Modbus RS485
  - 2.1 Signal transmission
  - 2.2 Supply voltage
- 3 Connection version: EtherNet/IP
  - 3.1 Signal transmission
  - 3.2 Supply voltage
- 4 Connection version: PROFIBUS DP
  - 4.1 PROFIBUS DP
  - 4.2 Supply voltage


**Transmitter**

Connection version 4-20 mA HART with pulse/frequency/switch output

Order code for "Output", option **B**

Depending on the housing version, the transmitters can be ordered with terminals or device plugs.

Order code for "Housing"	Connection methods available		Possible options for order code "Electrical connection"
	Outputs	Power supply	
Options A, B	Terminals	Terminals	<ul style="list-style-type: none"> <li>▪ Option A: coupling M20x1</li> <li>▪ Option B: thread M20x1</li> <li>▪ Option C: thread G ½"</li> <li>▪ Option D: thread NPT ½"</li> </ul>
Options A, B	Device plug	Terminals	<ul style="list-style-type: none"> <li>▪ Option L: plug M12x1 + thread NPT ½"</li> <li>▪ Option N: plug M12x1 + coupling M20</li> <li>▪ Option P: plug M12x1 + thread G ½"</li> <li>▪ Option U: plug M12x1 + thread M20</li> </ul>
Options A, B, C	Device plug	Device plug	Option Q: 2 x plug M12x1
Order code for "Housing": <ul style="list-style-type: none"> <li>▪ Option A: compact, coated aluminum</li> <li>▪ Option B: compact, hygienic, stainless</li> <li>▪ Option C: ultra compact, hygienic, stainless, M12 device plug</li> </ul>			

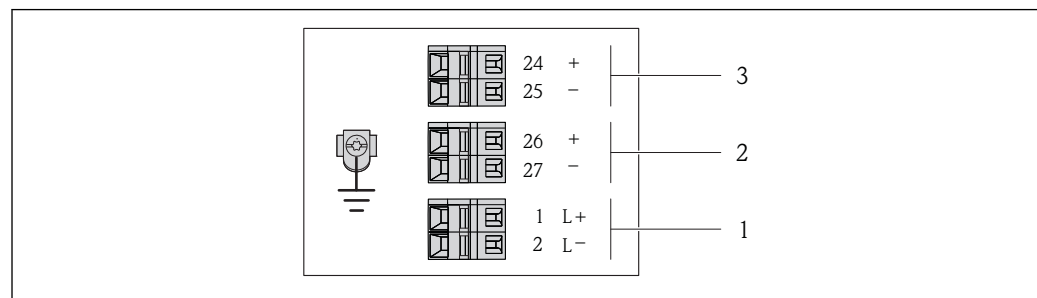

A0016888

2 Terminal assignment 4-20 mA HART with pulse/frequency/switch output

- 1 Power supply: DC 24 V
- 2 Output 1: 4-20 mA HART (active)
- 3 Output 2: pulse/frequency/switch output (passive)

Order code for "Output"	Terminal number					
	Power supply		Output 1		Output 2	
	2 (L-)	1 (L+)	27 (-)	26 (+)	25 (-)	24 (+)
Option B	DC 24 V		4-20 mA HART (active)		Pulse/frequency/switch output (passive)	
Order code for "Output": Option B: 4-20 mA HART with pulse/frequency/switch output						

*PROFIBUS DP connection version*

 For use in the non-hazardous area and Zone 2/Div. 2.


Order code for "Output", option **L**

Depending on the housing version, the transmitters can be ordered with terminals or device plugs.

Order code for "Housing"	Connection methods available		Possible options for order code "Electrical connection"
	Output	Power supply	
Options <b>A, B</b>	Terminals	Terminals	<ul style="list-style-type: none"> <li>▪ Option <b>A</b>: coupling M20x1</li> <li>▪ Option <b>B</b>: thread M20x1</li> <li>▪ Option <b>C</b>: thread G ½"</li> <li>▪ Option <b>D</b>: thread NPT ½"</li> </ul>
Options <b>A, B</b>	Device plug	Terminals	<ul style="list-style-type: none"> <li>▪ Option <b>L</b>: plug M12x1 + thread NPT ½"</li> <li>▪ Option <b>N</b>: plug M12x1 + coupling M20</li> <li>▪ Option <b>P</b>: plug M12x1 + thread G ½"</li> <li>▪ Option <b>U</b>: plug M12x1 + thread M20</li> </ul>
Options <b>A, B, C</b>	Device plug	Device plug	Option <b>Q</b> : 2 x plug M12x1

Order code for "Housing":

- Option **A**: compact, coated aluminum
- Option **A**: compact, hygienic, stainless
- Option **C**: ultra compact, hygienic, stainless, M12 device plug

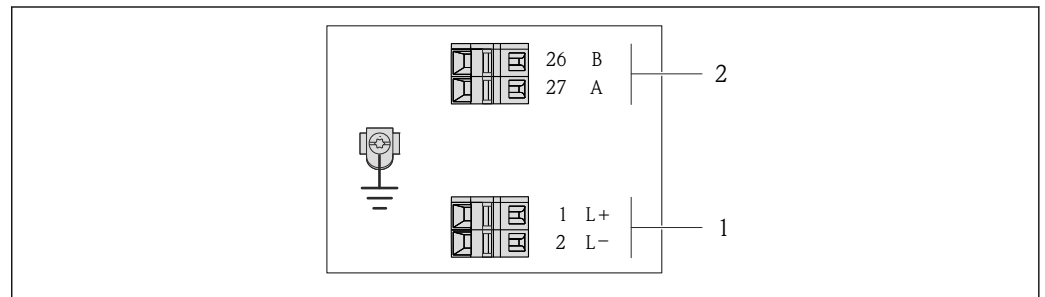

A0022716

 3 *PROFIBUS DP terminal assignment*

- 1 Power supply: DC 24 V
- 2 PROFIBUS DP

Order code for "Output"	Terminal number			
	Power supply		Output	
	2 (L-)	1 (L+)	26 (RxD/TxD-P)	27 (RxD/TxD-N)
Option <b>L</b>	DC 24 V		B	A

Order code for "Output":  
Option **L**: PROFIBUS DP, for use in non-hazardous areas and Zone 2/div. 2

Modbus RS485 connection version

 For use in the non-hazardous area and Zone 2/Div. 2.


Order code for "Output", option **M**

Depending on the housing version, the transmitters can be ordered with terminals or device plugs.


Order code for "Housing"	Connection methods available		Possible options for order code "Electrical connection"
	Output	Power supply	
Options A, B	Terminals	Terminals	<ul style="list-style-type: none"> <li>▪ Option A: coupling M20x1</li> <li>▪ Option B: thread M20x1</li> <li>▪ Option C: thread G ½"</li> <li>▪ Option D: thread NPT ½"</li> </ul>
Options A, B	Device plug	Terminals	<ul style="list-style-type: none"> <li>▪ Option L: plug M12x1 + thread NPT ½"</li> <li>▪ Option N: plug M12x1 + coupling M20</li> <li>▪ Option P: plug M12x1 + thread G ½"</li> <li>▪ Option U: plug M12x1 + thread M20</li> </ul>
Options A, B, C	Device plug	Device plug	Option Q: 2 x plug M12x1

Order code for "Housing":

- Option A: compact, coated aluminum
- Option B: compact, hygienic, stainless
- Option C: ultra compact, hygienic, stainless, M12 device plug
- Option C: ultra compact, stainless, M12 device plug

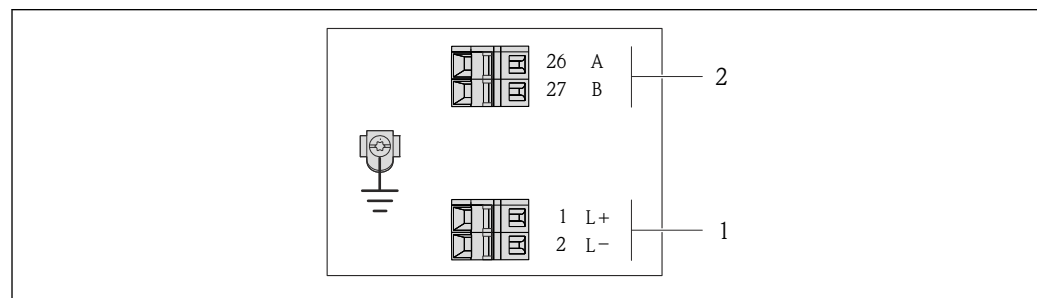

A0019528

 4 Modbus RS485 terminal assignment, connection version for use in non-hazardous areas and Zone 2/Div. 2

- 1 Power supply: DC 24 V
- 2 Modbus RS485

Order code for "Output"	Terminal number			
	Power supply		Output	
	2 (L-)	1 (L+)	27 (B)	26 (A)
Option <b>M</b>	DC 24 V		Modbus RS485	

Order code for "Output":  
Option **M**: Modbus RS485, for use in non-hazardous areas and Zone 2/Div. 2

*Modbus RS485 connection version*

 For use in the intrinsically safe area. Connection via Safety Barrier Promass 100.


Order code for "Output", option **M**

Depending on the housing version, the transmitters can be ordered with terminals or device plugs.


Order code for "Housing"	Connection methods available		Possible options for order code "Electrical connection"
	Output	Power supply	
Options A, B	Terminals	Terminals	<ul style="list-style-type: none"> <li>▪ Option A: coupling M20x1</li> <li>▪ Option B: thread M20x1</li> <li>▪ Option C: thread G ½"</li> <li>▪ Option D: thread NPT ½"</li> </ul>
A, B, C	Device plug		Option I: plug M12x1

Order code for "Housing":

- Option A: compact, coated aluminum
- Option B: compact, hygienic, stainless
- Option C: ultra compact, hygienic, stainless, M12 device plug

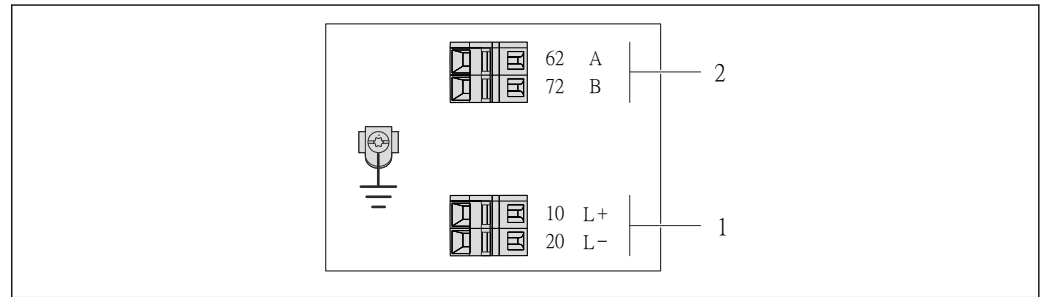

A0017053

 5 *Modbus RS485 terminal assignment, connection version for use in intrinsically safe areas (connection via Safety Barrier Promass 100)*

- 1 *Intrinsically safe power supply*
- 2 *Modbus RS485*

Order code for "Output"	20 (L-)	10 (L+)	72 (B)	62 (A)
Option <b>M</b>	Intrinsically safe supply voltage		Modbus RS485 intrinsically safe	

Order code for "Output":  
 Option **M**: Modbus RS485, for use in intrinsically safe areas (connection via Safety Barrier Promass 100)

*EtherNet/IP connection version*


Order code for "Output", option **N**

Depending on the housing version, the transmitters can be ordered with terminals or device plugs.

Order code for "Housing"	Connection methods available		Possible options for order code "Electrical connection"
	Output	Power supply	
Options <b>A, B</b>	Device plug	Terminals	<ul style="list-style-type: none"> <li>▪ Option <b>L</b>: plug M12x1 + thread NPT ½"</li> <li>▪ Option <b>N</b>: plug M12x1 + coupling M20</li> <li>▪ Option <b>P</b>: plug M12x1 + thread G ½"</li> <li>▪ Option <b>U</b>: plug M12x1 + thread M20</li> </ul>
Options <b>A, B, C</b>	Device plug	Device plug	Option <b>Q</b> : 2 x plug M12x1

Order code for "Housing":

- Option **A**: compact, coated aluminum
- Option **B**: compact, hygienic, stainless
- Option **C**: ultra compact, hygienic, stainless, M12 device plug

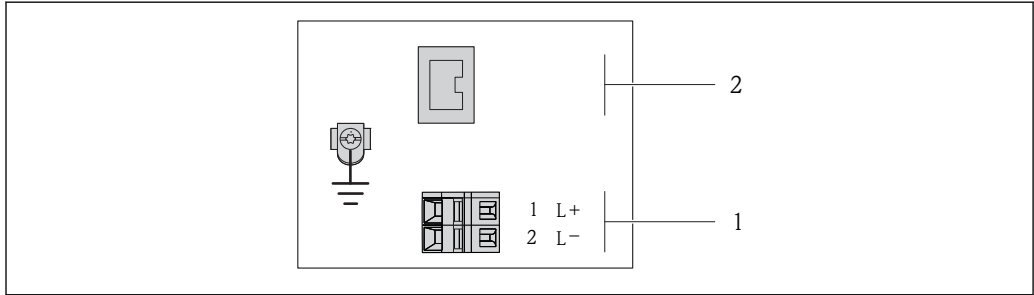

A0017054

6 EtherNet/IP terminal assignment


- 1 Power supply: DC 24 V
- 2 EtherNet/IP

Order code for "Output"	Terminal number		Output Device plug M12x1
	Power supply 2 (L-)	1 (L+)	
Option <b>N</b>	DC 24 V		EtherNet/IP

Order code for "Output":  
Option **N**: EtherNet/IP



**Safety Barrier Promass 100**

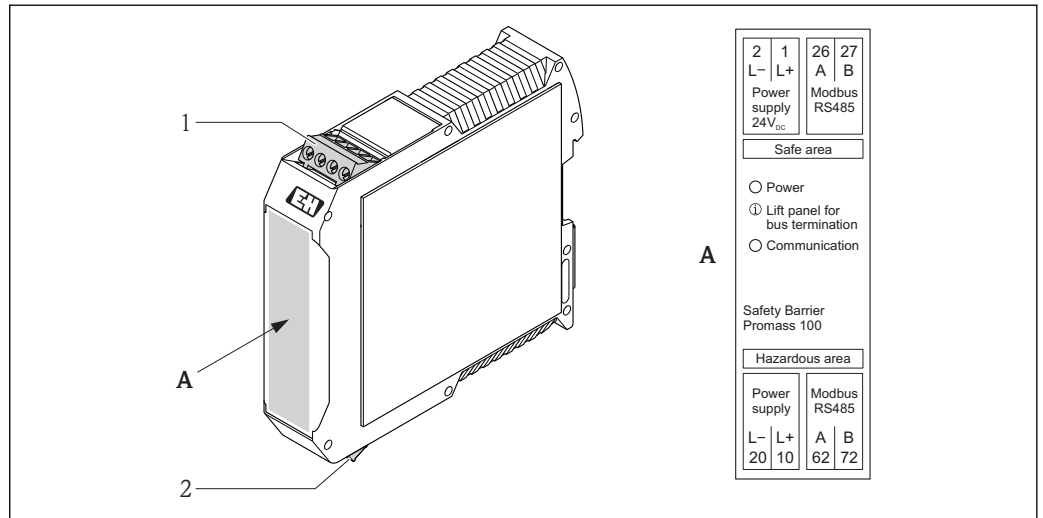

7 Safety Barrier Promass 100 with terminals

- 1 Non-hazardous area and Zone 2/Div. 2
- 2 Intrinsically safe area

A0016922

**Pin assignment, device plug**

- i** Order codes for the M12x1 connectors, see the "Order code for **electrical connection**" column:
  - 4-20 mA HART, pulse/frequency/switch output (→ 19)
  - PROFIBUS-DP (→ 21)
  - Modbus RS485 (→ 22)
  - EtherNet/IP (→ 24)

**Supply voltage**

For all connection versions except MODBUS RS485 intrinsically safe (device side)


- i** Device plug MODBUS RS485 intrinsically safe with supply voltage (→ 26)


	Pin	Assignment	Coding	Plug/socket	
<p>A0016809</p>	1	L+	A	Plug	
	2				
	3				
	4	L-			DC 24 V
	5				Grounding/shielding

- i** The following is recommended as a socket:
  - Binder, series 763, part no. 79 3440 35 05
  - Alternatively: Phoenix part no. 1669767 SAC-5P-M12MS
    - With the order code for "Output", option **B**: 4-20 mA HART, pulse/frequency/switch output
    - With the order code for "Output", option **N**: EtherNet/IP
  - When using the device in a hazardous location: Use a suitably certified socket.

#### 4-20 mA HART with pulse/frequency/switch output

Device plug for signal transmission (device side)


	Pin		Assignment	Coding	Plug/socket
	1	+	4-20 mA HART (active)	A	Socket
	2	-	4-20 mA HART (active)		
	3	+	Pulse/frequency/switch output (passive)		
	4	-	Pulse/frequency/switch output (passive)		
	5		Grounding/shielding		

-  Recommended plug: Binder, series 763, part no. 79 3439 12 05
-  When using the device in a hazardous location: Use a suitably certified plug.

#### PROFIBUS DP

-  For use in the non-hazardous area and Zone 2/Div. 2.


Device plug for signal transmission (device side)



	Pin		Assignment	Coding	Plug/socket
	1			B	Socket
	2	A	PROFIBUS DP		
	3				
	4	B	PROFIBUS DP		
	5		Grounding/shielding		

-  Recommended plug: Binder, series 763, part no. 79 4449 20 05
-  When using the device in a hazardous location: Use a suitably certified plug.

#### MODBUS RS485

Device plug for signal transmission with supply voltage (device side), MODBUS RS485 (intrinsically safe)

	Pin		Assignment	Coding	Plug/socket
	1	L+	Supply voltage, intrinsically safe	A	Plug
	2	A	Modbus RS485 intrinsically safe		
	3	B			
	4	L-	Supply voltage, intrinsically safe		
	5		Grounding/shielding		

-  Recommended socket: Binder, series 763, part no. 79 3439 12 05
-  When using the device in a hazardous location: Use a suitably certified socket.

Device plug for signal transmission (device side), MODBUS RS485 (not intrinsically safe)

**i** For use in the non-hazardous area and Zone 2/Div. 2.

	Pin	Assignment	Coding	Plug/socket	
	1			B	Socket
	2	A	Modbus RS485		
	3				
	4	B	Modbus RS485		
5		Grounding/shielding			

- i** Recommended plug: Binder, series 763, part no. 79 4449 20 05
- When using the device in a hazardous location: Use a suitably certified plug.

**EtherNet/IP**

Device plug for signal transmission (device side)

	Pin	Assignment	Coding	Plug/socket	
	1	+	Tx	D	Socket
	2	+	Rx		
	3	-	Tx		
	4	-	Rx		

- i** Recommended plug:
  - Binder, series 763, part no. 99 3729 810 04
  - Phoenix, part no. 1543223 SACC-M12MSD-4Q
  - When using the device in a hazardous location: Use a suitably certified plug.

**Supply voltage**

**Transmitter**

- For device version with all communication types except Modbus RS485 intrinsically safe: DC 20 to 30 V
- For device version with Modbus RS485 intrinsically safe: power supply via Safety Barrier Promass 100

The power unit must be tested to ensure it meets safety requirements (e.g. PELV, SELV).

**Safety Barrier Promass 100**

DC 20 to 30 V

**Power consumption**

*Transmitter*

Order code for "Output"	Maximum Power consumption
Option <b>B</b> : 4-20mA HART, pulse/frequency/switch output	3.5 W
Option <b>L</b> : PROFIBUS DP	3.5 W
Option <b>M</b> : Modbus RS485, for use in non-hazardous areas and Zone 2/Div. 2	3.5 W
Option <b>M</b> : Modbus RS485, for use in intrinsically safe areas	2.45 W
Option <b>N</b> : EtherNet/IP	3.5 W

## Safety Barrier Promass 100

Order code for "Output"	Maximum Power consumption
Option <b>M</b> : Modbus RS485, for use in intrinsically safe areas	4.8 W

## Current consumption

## Transmitter

Order code for "Output"	Maximum Current consumption	Maximum switch-on current
Option <b>B</b> : 4-20mA HART, pul./freq./switch output	145 mA	18 A (<0.125 ms)
Option <b>L</b> : PROFIBUS DP	145 mA	18 A (<0.125 ms)
Option <b>M</b> : Modbus RS485, for use in non-hazardous areas and Zone 2/Div. 2	90 mA	10 A (<0.8 ms)
Option <b>M</b> : Modbus RS485, for use in intrinsically safe areas	145 mA	16 A (<0.4 ms)
Option <b>N</b> : EtherNet/IP	145 mA	18 A (<0.125 ms)

## Safety Barrier Promass 100


Order code for "Output"	Maximum Current consumption	Maximum switch-on current
Option <b>M</b> : Modbus RS485, for use in intrinsically safe areas	230 mA	10 A (<0.8 ms)

## Power supply failure

- Totalizers stop at the last value measured.
- Depending on the device version, the configuration is retained in the device memory or in the plug-in memory (HistoROM DAT).
- Error messages (incl. total operated hours) are stored.

## Electrical connection

## Connecting the transmitter

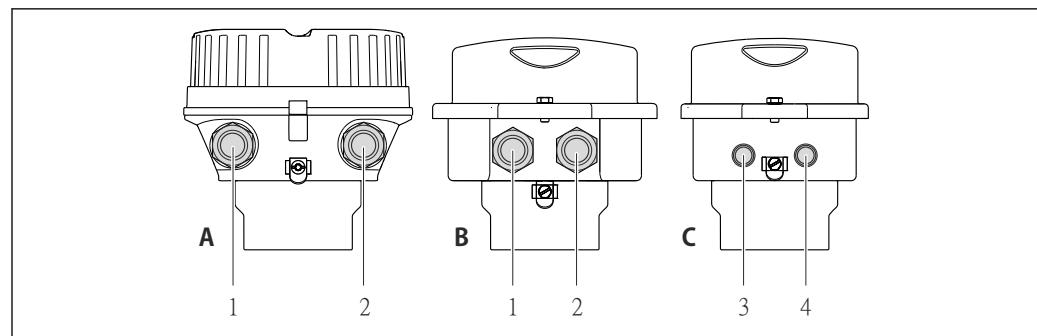

A0016924


- A Housing version: compact, aluminum coated  
 B Housing version: compact hygienic, stainless  
 1 Cable entry or device plug for signal transmission  
 2 Cable entry or device plug for supply voltage  
 C Housing version: ultra-compact hygienic, stainless, M12 device plug  
 3 Device plug for signal transmission  
 4 Device plug for supply voltage

- Terminal assignment (→ 19)
- Pin assignment, device plug (→ 25)

- In the case of device versions with a connector, the transmitter housing does not need to be opened to connect the signal cable or power supply cable.

Connection examples


Current output 4-20 mA HART

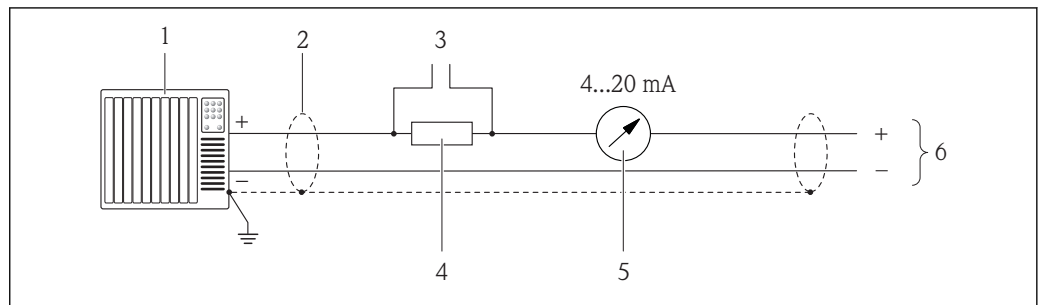

8 Connection example for 4-20 mA HART current output (active)

- 1 Automation system with current input (e.g. PLC)
- 2 Cable shield, observe cable specifications (→ 33)
- 3 Connection for HART operating devices (→ 74)
- 4 Resistor for HART communication ( $\geq 250 \Omega$ ): observe maximum load (→ 9)
- 5 Analog display unit: observe maximum load (→ 9)
- 6 Transmitter


Pulse/frequency output

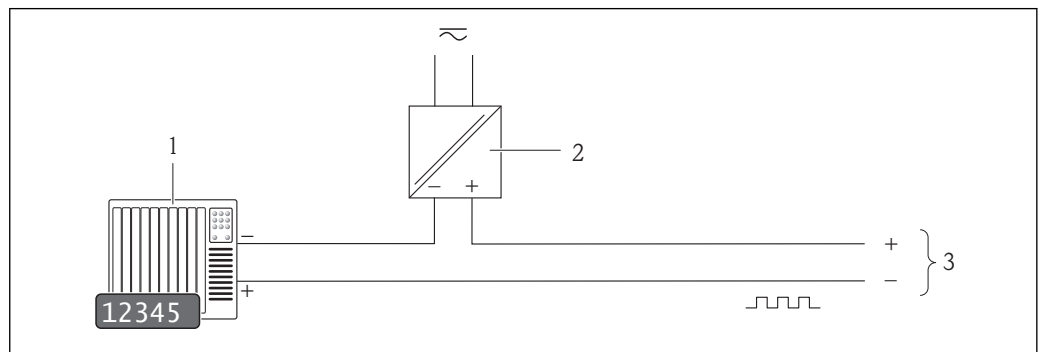

9 Connection example for pulse/frequency output (passive)

- 1 Automation system with pulse/frequency input (e.g. PLC)
- 2 Power supply
- 3 Transmitter: observe input values (→ 9)


Switch output

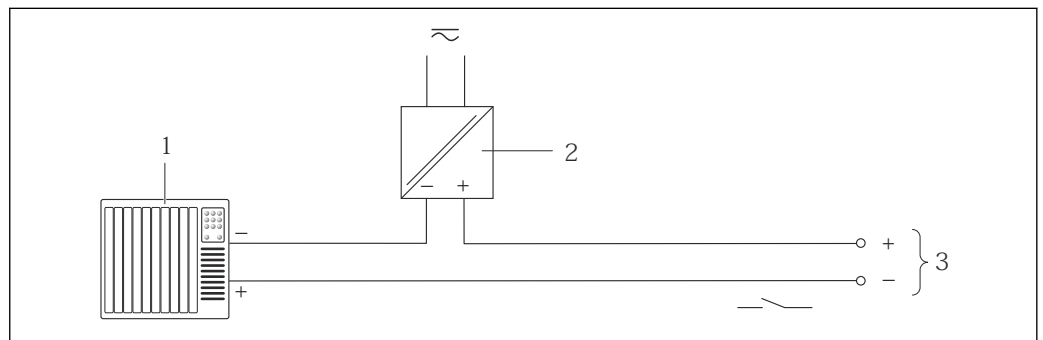

10 Connection example for switch output (passive)

- 1 Automation system with switch input (e.g. PLC)
- 2 Power supply
- 3 Transmitter: observe input values (→ 9)

## PROFIBUS DP

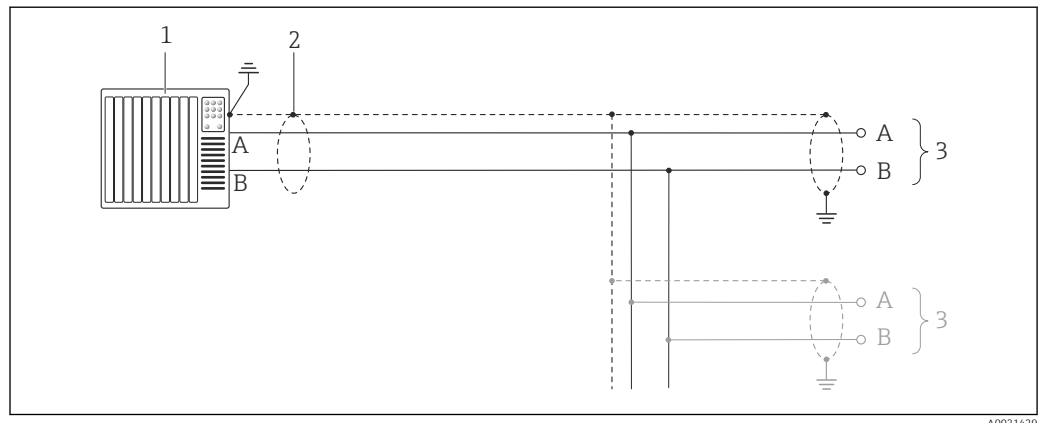


A0021429

11 Connection example for PROFIBUS DP, non-hazardous area and Zone 2/Div. 2

- 1 Control system (e.g. PLC)
- 2 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications (→ 33)
- 3 Distribution box
- 4 Transmitter

**i** If baud rates > 1.5 MBaud an EMC cable entry must be used and the cable shield must continue as far as the terminal wherever possible.


## Modbus RS485

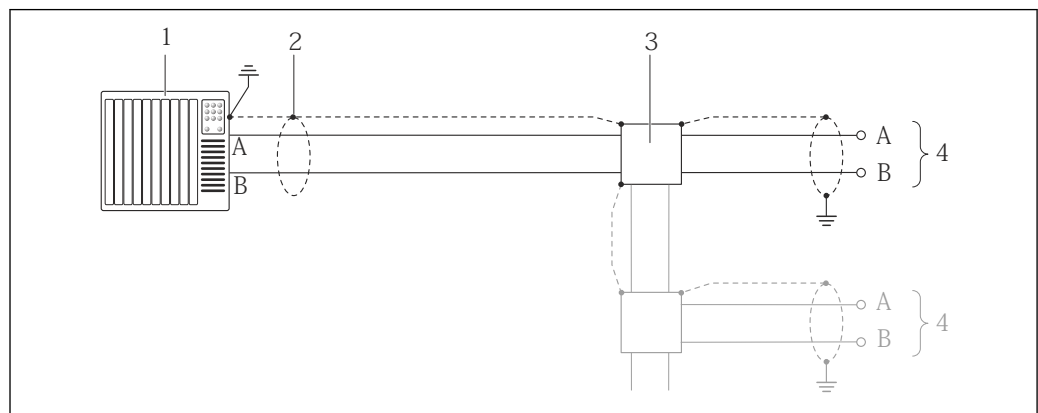

A0016803

12 Connection example for Modbus RS485, non-hazardous area and Zone 2/Div. 2

- 1 Control system (e.g. PLC)
- 2 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications (→ 33)
- 3 Distribution box
- 4 Transmitter

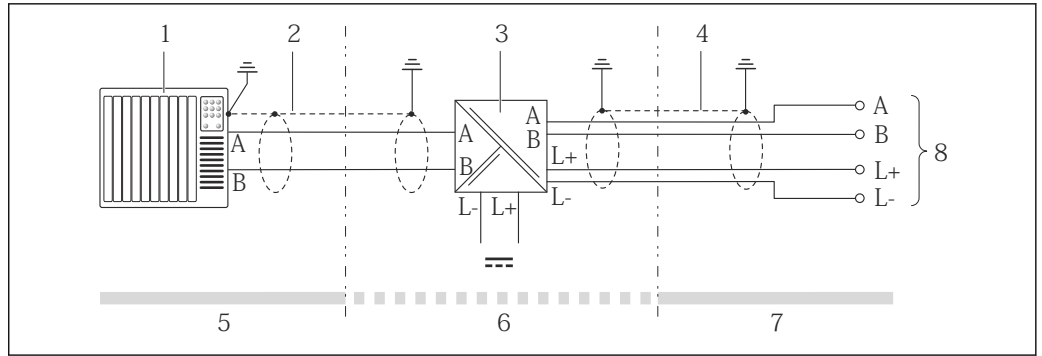


A0016804

13 Connection example for Modbus RS485 intrinsically safe

- 1 Control system (e.g. PLC)
- 2 Cable shield, observe cable specifications (→ 33)
- 3 Safety Barrier Promass 100
- 4 Observe cable specifications (→ 33)
- 5 Non-hazardous area
- 6 Non-hazardous area and Zone 2/Div. 2
- 7 Intrinsically safe area
- 8 Transmitter

EtherNet/IP

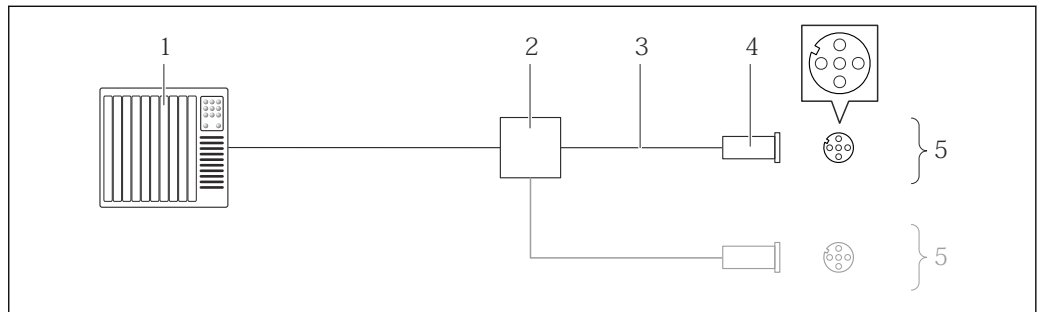


A0016805

14 Connection example for EtherNet/IP

- 1 Control system (e.g. PLC)
- 2 Ethernet switch
- 3 Observe cable specifications (→ 33)
- 4 Connector
- 5 Transmitter


## HART input

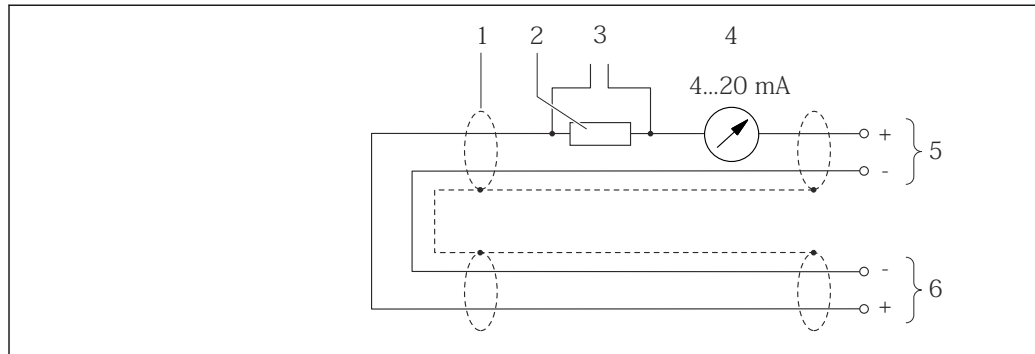

A0019826

15 Connection example for HART input (burst mode) via current output (active)

- 1 Cable shield, observe cable specifications (→ 33)
- 2 Resistor for HART communication ( $\geq 250 \Omega$ ): observe maximum load (→ 9)
- 3 Connection for HART operating devices (→ 74)
- 4 Analog display unit
- 5 Transmitter
- 6 Sensor for external measured variable

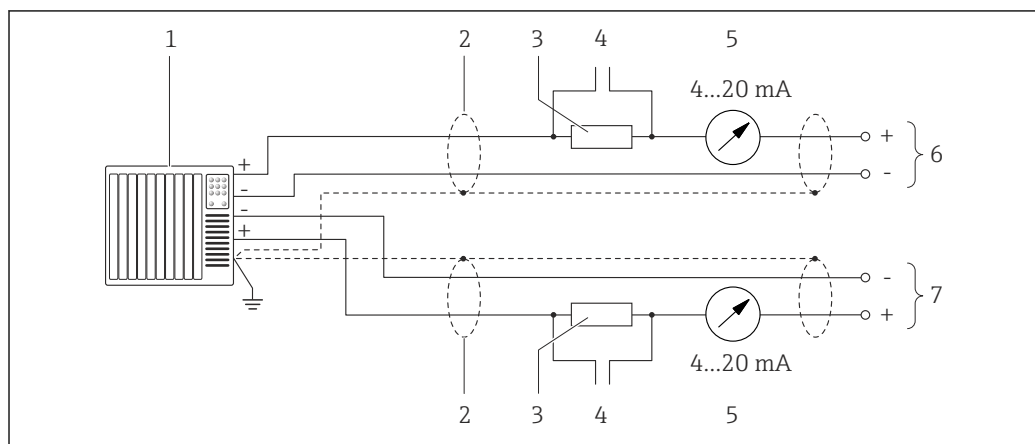

A0019830

16 Connection example for HART input (master mode) via current output (active)

- 1 Automation system with current input (e.g. PLC).  
Prerequisite: automation system with HART version 6, HART commands 113 and 114 can be processed.
- 2 Cable shield, observe cable specifications (→ 33)
- 3 Resistor for HART communication ( $\geq 250 \Omega$ ): observe maximum load (→ 9)
- 4 Connection for HART operating devices (→ 74)
- 5 Analog display unit
- 6 Transmitter
- 7 Sensor for external measured variable

## Potential equalization

No special measures for potential equalization are required.



For devices intended for use in hazardous locations, please observe the guidelines in the Ex documentation (XA).

## Terminals

## Transmitter

Spring terminals for wire cross-sections  $0.5$  to  $2.5 \text{ mm}^2$  (20 to 14 AWG)

## Safety Barrier Promass 100

Plug-in screw terminals for wire cross-sections  $0.5$  to  $2.5 \text{ mm}^2$  (20 to 14 AWG)



**Cable entries**

- Cable gland: M20 × 1.5 with cable  $\phi$ 6 to 12 mm (0.24 to 0.47 in)
- Thread for cable entry:
  - NPT 1/2"
  - G 1/2"
  - M20

**Cable specification**

**Permitted temperature range**

- -40 °C (-40 °F) to +80 °C (+176 °F)
- Minimum requirement: cable temperature range  $\geq$  ambient temperature +20 K

**Power supply cable**

Standard installation cable is sufficient.

**Signal cable**

*Current output*

For 4-20 mA HART: Shielded cable recommended. Observe grounding concept of the plant.

*Pulse/frequency/switch output*

Standard installation cable is sufficient.

*PROFIBUS DP*

The IEC 61158 standard specifies two types of cable (A and B) for the bus line which can be used for every transmission rate. Cable type A is recommended.

<b>Cable type</b>	A
<b>Characteristic impedance</b>	135 to 165 $\Omega$ at a measuring frequency of 3 to 20 MHz
<b>Cable capacitance</b>	<30 pF/m
<b>Wire cross-section</b>	>0.34 mm <sup>2</sup> (22 AWG)
<b>Cable type</b>	Twisted pairs
<b>Loop resistance</b>	$\leq$ 110 $\Omega$ /km
<b>Signal damping</b>	Max. 9 dB over the entire length of the cable cross-section
<b>Shielding</b>	Copper braided shielding or braided shielding with foil shield. When grounding the cable shield, observe the grounding concept of the plant.


*Modbus RS485*

The EIA/TIA-485 standard specifies two types of cable (A and B) for the bus line which can be used for every transmission rate. Cable type A is recommended.

<b>Cable type</b>	A
<b>Characteristic impedance</b>	135 to 165 $\Omega$ at a measuring frequency of 3 to 20 MHz
<b>Cable capacitance</b>	<30 pF/m
<b>Wire cross-section</b>	>0.34 mm <sup>2</sup> (22 AWG)
<b>Cable type</b>	Twisted pairs
<b>Loop resistance</b>	$\leq$ 110 $\Omega$ /km
<b>Signal damping</b>	Max. 9 dB over the entire length of the cable cross-section
<b>Shielding</b>	Copper braided shielding or braided shielding with foil shield. When grounding the cable shield, observe the grounding concept of the plant.

*EtherNet/IP*


The standard ANSI/TIA/EIA-568-B.2 Annex specifies CAT 5 as the minimum category for a cable used for EtherNet/IP. CAT 5e and CAT 6 are recommended.

 For more information on planning and installing EtherNet/IP networks, please refer to the "Media Planning and Installation Manual. EtherNet/IP" of the ODVA Organization.

### Connecting cable between Safety Barrier Promass 100 and measuring device

<b>Cable type</b>	Shielded twisted-pair cable with 2x2 wires. When grounding the cable shield, observe the grounding concept of the plant.
<b>Maximum cable resistance</b>	2.5 Ω, one side

► Comply with the maximum cable resistance specifications to ensure the operational reliability of the measuring device.



The maximum cable length for individual wire cross-sections is specified in the table below. Observe the maximum capacitance and inductance per unit length of the cable and connection values for hazardous areas (→  12).

Wire cross-section		Maximum cable length	
[mm <sup>2</sup> ]	[AWG]	[m]	[ft]
0.5	20	70	230
0.75	18	100	328
1.0	17	100	328
1.5	16	200	656
2.5	14	300	984

## Performance characteristics

### Reference operating conditions

- Error limits based on ISO 11631
- Water with +15 to +45 °C (+59 to +113 °F) at 2 to 6 bar (29 to 87 psi)
- Specifications as per calibration protocol
- Accuracy based on accredited calibration rigs that are traced to ISO 17025.

 To obtain measured errors, use the *Applicator* sizing tool (→  82)

### Maximum measured error

o.r. = of reading; 1 g/cm<sup>3</sup> = 1 kg/l; T = medium temperature

#### Base accuracy

#### Mass flow and volume flow (liquids)

±0.10 %

#### Mass flow (gases)

±0.50 % o.r.

 Design fundamentals (→  37)

#### Density (liquids)

- Reference conditions: ±0.0005 g/cm<sup>3</sup>
- Standard density calibration: ±0.02 g/cm<sup>3</sup>  
(valid over the entire temperature range and density range)
- Wide-range density specification (order code for "Application package", option EF "Special density and concentration" or EH "Special density and viscosity"): ±0.004 g/cm<sup>3</sup> (valid range for special density calibration: 0 to 2 g/cm<sup>3</sup>, +10 to +80 °C (+50 to +176 °F))

#### Temperature

±0.5 °C ± 0.005 · T °C (±0.9 °F ± 0.003 · (T - 32) °F)

**Zero point stability**

DN		Zero point stability	
[mm]	[in]	[kg/h]	[lb/min]
8	$\frac{3}{8}$	0.150	0.0055
15	$\frac{1}{2}$	0.488	0.0179
15 FB	$\frac{1}{2}$ FB	1.350	0.0496
25	1	1.350	0.0496
25 FB	1 FB	3.375	0.124
40	$1\frac{1}{2}$	3.375	0.124
40 FB	$1\frac{1}{2}$ FB	5.25	0.193
50	2	5.25	0.193
50 FB	2 FB	13.5	0.496
80	3	13.5	0.496

FB = Full bore

**Flow values**

Flow values as turndown parameter depending on nominal diameter.

*SI units*

DN	1:1	1:10	1:20	1:50	1:100	1:500
	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]	[kg/h]
8	2 000	200	100	40	20	4
15	6 500	650	325	130	65	13
15 FB	18 000	1 800	900	360	180	36
25	18 000	1 800	900	360	180	36
25 FB	45 000	4 500	2 250	900	450	90
40	45 000	4 500	2 250	900	450	90
40 FB	70 000	7 000	3 500	1 400	700	140
50	70 000	7 000	3 500	1 400	700	140
50 FB	180 000	18 000	9 000	3 600	1 800	360
80	180 000	18 000	9 000	3 600	1 800	360

FB = Full bore

*US units*


DN	1:1	1:10	1:20	1:50	1:100	1:500
	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]
$\frac{3}{8}$	73.50	7.350	3.675	1.470	0.735	0.147
$\frac{1}{2}$	238.9	23.89	11.95	4.778	2.389	0.478
$\frac{1}{2}$ FB	661.5	66.15	33.08	13.23	6.615	1.323
1	661.5	66.15	33.08	13.23	6.615	1.323
1 FB	1 654	165.4	82.70	33.08	16.54	3.308
$1\frac{1}{2}$	1 654	165.4	82.70	33.08	16.54	3.308
$1\frac{1}{2}$ FB	2 573	257.3	128.7	51.46	25.73	5.146

DN	1:1	1:10	1:20	1:50	1:100	1:500
[inch]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]	[lb/min]
2	2 573	257.3	128.7	51.46	25.73	5.146
2 FB	6 615	661.5	330.8	132.3	66.15	13.23
3	6 615	661.5	330.8	132.3	66.15	13.23

FB = Full bore

### Accuracy of outputs

o.r. = of reading; o.f.s. = of full scale value

 The output accuracy must be factored into the measured error if analog outputs are used, but can be ignored for fieldbus outputs (e.g. Modbus RS485, EtherNet/IP).

#### Current output

Accuracy	Max. $\pm 0.05$ % o.f.s. or $\pm 5$ $\mu$ A
----------	---

#### Pulse/frequency output

Accuracy	Max. $\pm 50$ ppm o.r.
----------	------------------------

### Repeatability

o.r. = of reading;  $1 \text{ g/cm}^3 = 1 \text{ kg/l}$ ; T = medium temperature

#### Base repeatability

##### Mass flow and volume flow (liquids)

$\pm 0.05$  % o.r.

##### Mass flow (gases)

$\pm 0.25$  % o.r.

 Design fundamentals ([→](#)  37)

##### Density (liquids)

$\pm 0.00025 \text{ g/cm}^3$

##### Temperature

$\pm 0.25 \text{ }^\circ\text{C} \pm 0.0025 \cdot T \text{ }^\circ\text{C}$  ( $\pm 0.45 \text{ }^\circ\text{F} \pm 0.0015 \cdot (T-32) \text{ }^\circ\text{F}$ )

### Response time

The response time depends on the configuration (damping).

### Influence of ambient temperature

o.r. = of reading; o.f.s. = of full scale value

#### Current output

Temperature coefficient	Max. $\pm 50$ ppm/ $^\circ\text{C}$ o.f.s. or $\pm 1$ $\mu$ A/ $^\circ\text{C}$
-------------------------	---

#### Pulse/frequency output

Temperature coefficient	Max. $\pm 50$ ppm o.r. / $100 \text{ }^\circ\text{C}$
-------------------------	---

### Influence of medium temperature


#### Mass flow and volume flow


When there is a difference between the temperature for zero point adjustment and the process temperature, the typical measured error of the sensor is  $\pm 0.0002$  % of the full scale value/ $^\circ\text{C}$  ( $\pm 0.0001$  % of the full scale value/ $^\circ\text{F}$ ).

#### Density

When there is a difference between the density calibration temperature and the process temperature, the typical measured error of the sensor is  $\pm 0.0001 \text{ g/cm}^3 \text{ }^\circ\text{C}$  ( $\pm 0.00005 \text{ g/cm}^3 \text{ }^\circ\text{F}$ ). Field density calibration is possible.

**Wide-range density specification (special density calibration)**

If the process temperature is outside the valid range ( $\rightarrow$   34) the measured error is  $\pm 0.0001 \text{ g/cm}^3 / ^\circ\text{C}$  ( $\pm 0.00005 \text{ g/cm}^3 / ^\circ\text{F}$ )

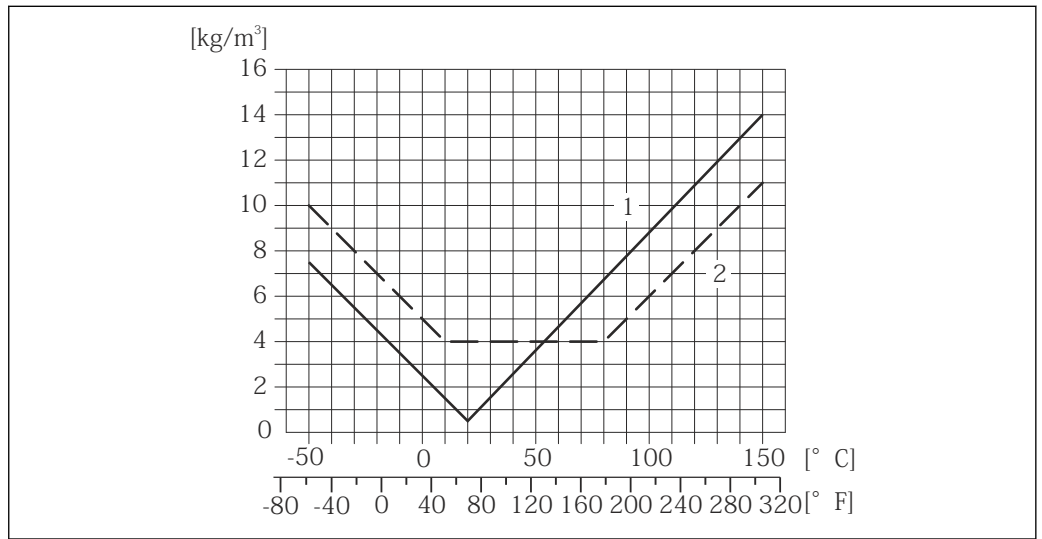

A0016614

- 1 Field density calibration, for example at +20 °C (+68 °F)
- 2 Special density calibration

**Temperature**

$\pm 0.005 \cdot T \text{ } ^\circ\text{C}$  ( $\pm 0.005 \cdot (T - 32) \text{ } ^\circ\text{F}$ )

**Influence of medium pressure**

The table below shows the effect on accuracy of mass flow due to a difference between calibration pressure and process pressure.

o.r. = of reading

DN		[% o.r./bar]	[% o.r./psi]
[mm]	[in]		
8	3/8	no influence	no influence
15	1/2	no influence	no influence
15 FB	1/2 FB	-0.003	-0.0002
25	1	-0.003	-0.0002
25 FB	1 FB	no influence	no influence
40	1 1/2	no influence	no influence
40 FB	1 1/2 FB	no influence	no influence
50	2	no influence	no influence
50 FB	2 FB	-0.003	-0.0002
80	3	no influence	no influence
FB = Full bore			

**Design fundamentals**

o.r. = of reading, o.f.s. = of full scale value

BaseAccu = base accuracy in % o.r., BaseRepeat = base repeatability in % o.r.

MeasValue = measured value; ZeroPoint = zero point stability


Calculation of the maximum measured error as a function of the flow rate

Flow rate	Maximum measured error in % o.r.
$\geq \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$ A0021332	$\pm \text{BaseAccu}$ A0021339
$< \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$ A0021333	$\pm \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$ A0021334

Calculation of the maximum repeatability as a function of the flow rate

Flow rate	Maximum repeatability in % o.r.
$\geq \frac{1/2 \cdot \text{ZeroPoint}}{\text{BaseRepeat}} \cdot 100$ A0021335	$\pm \text{BaseRepeat}$ A0021340
$< \frac{1/2 \cdot \text{ZeroPoint}}{\text{BaseRepeat}} \cdot 100$ A0021336	$\pm 1/2 \cdot \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$ A0021337

### Example for max. measured error

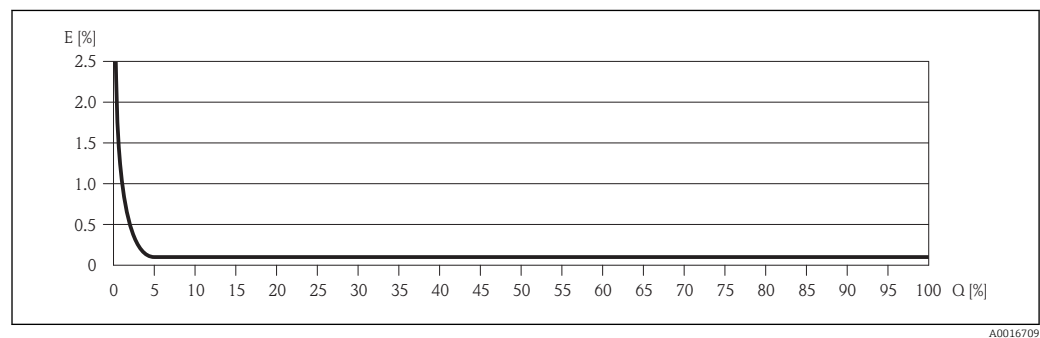

*E* Error: Maximum measured error as % o.r. (example)

*Q* Flow rate as %



Design fundamentals (→ 37)


## Installation

No special measures such as supports are necessary. External forces are absorbed by the construction of the device.

### Mounting location

To prevent measuring errors arising from accumulation of gas bubbles in the measuring tube, avoid the following mounting locations in the pipe:


- Highest point of a pipeline.
- Directly upstream of a free pipe outlet in a down pipe.

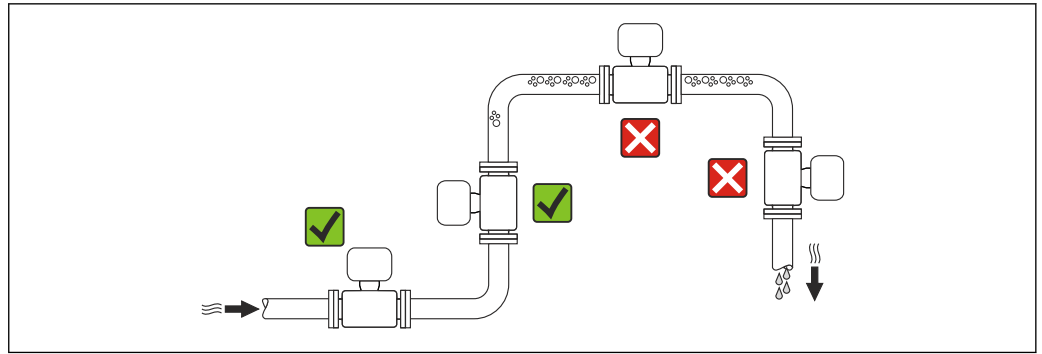

A0023344

**Installation in down pipes**

However, the following installation suggestion allows for installation in an open vertical pipeline. Pipe restrictions or the use of an orifice with a smaller cross-section than the nominal diameter prevent the sensor running empty while measurement is in progress.

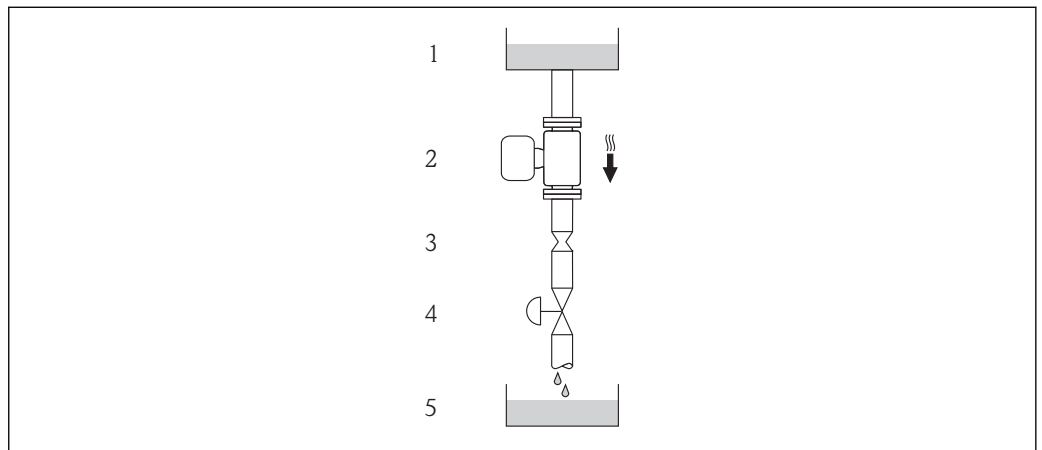

A0015596

17 Installation in a down pipe (e.g. for batching applications)





- 1 Supply tank
- 2 Sensor
- 3 Orifice plate, pipe restriction
- 4 Valve
- 5 Batching tank

DN		Ø orifice plate, pipe restriction	
[mm]	[in]	[mm]	[in]
8	3/8	6	0.24
15	1/2	10	0.40
15 FB	1/2 FB	15	0.60
25	1	14	0.55
25 FB	1 FB	24	0.95
40	1 1/2	22	0.87
40 FB	1 1/2 FB	35	1.38
50	2	28	1.10
50 FB	2 FB	54	2.13
80	3	50	1.97

FB = Full bore

**Orientation**

The direction of the arrow on the sensor nameplate helps you to install the sensor according to the flow direction (direction of medium flow through the piping).

Orientation		Recommendation	
<b>A</b>	Vertical orientation	 A0015591	☑☑
<b>B</b>	Horizontal orientation, transmitter head up	 A0015589	☑☑ <sup>1)</sup> Exception:
<b>C</b>	Horizontal orientation, transmitter head down	 A0015590	☑☑ <sup>2)</sup> Exception:
<b>D</b>	Horizontal orientation, transmitter head at side	 A0015592	☑☑(→ ☑ 40)


- 1) Applications with low process temperatures may reduce the ambient temperature. To maintain the minimum ambient temperature for the transmitter, this orientation is recommended.
- 2) Applications with high process temperatures may increase the ambient temperature. To maintain the maximum ambient temperature for the transmitter, this orientation is recommended.

**Inlet and outlet runs**

No special precautions need to be taken for fittings which create turbulence, such as valves, elbows or T-pieces, as long as no cavitation occurs (→ ☑ 49).

**Special mounting instructions****Guarantees complete drainability**

When the sensor is installed in a horizontal line, eccentric clamps can be used to ensure complete drainability. When the system is pitched in a specific direction and at a specific slope, gravity can be used to achieve complete drainability. The sensor must be mounted in the correct position to ensure full drainability in the horizontal position. Markings on the sensor show the correct mounting position to optimize drainability.

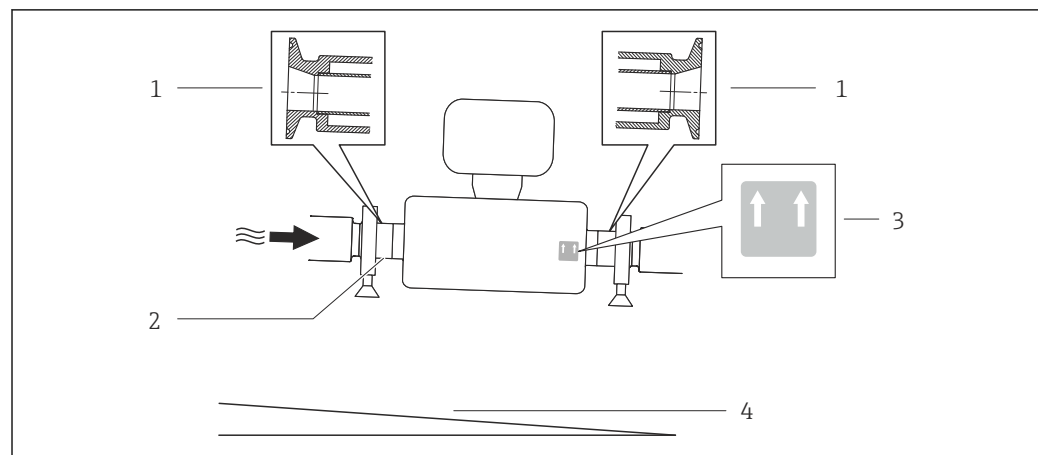

A0016585

☑ 18


- 1 Eccentric clamp connection
- 2 Line on the underside indicates the lowest point of the eccentric process connection.
- 3 "This side up" label indicates which side is up
- 4 Slope the device in accordance with the hygiene guidelines. Slope: approx. 2 % or 21mm/m (0.24 in/feet)



**Securing with mounting clamp in the case of hygiene connections**

It is not necessary to provide additional support for the sensor for operational performance purposes. If, however, additional support is required for installation purposes, the following dimensions must be observed.

Use mounting clamp with lining between clamp and measuring instrument.

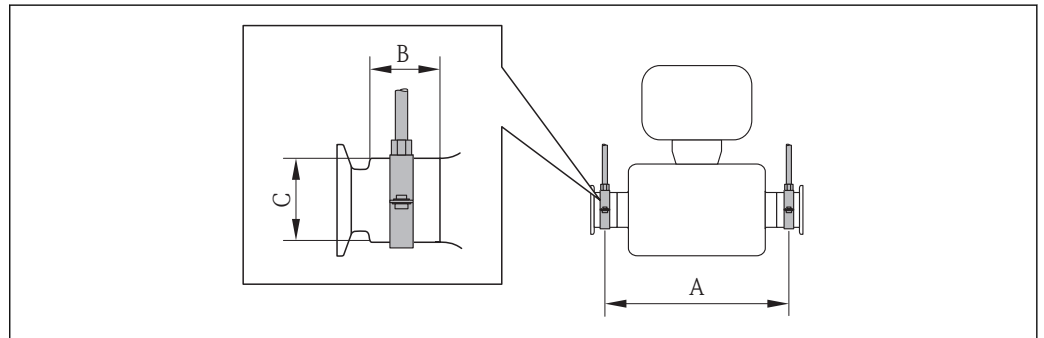

A0016588

*SI units*

DN [mm]	8	15	15 FB	25	25 FB	40	40 FB	50	50 FB	80
A [mm]	373	409	539	539	668	668	780	780	1152	1152
B [mm]	20	20	30	30	28	28	35	35	57	57
C [mm]	40	40	44.5	44.5	60	60	80	80	90	90

*US units*

DN [in]	3/8	1/2	1/2 FB	1	1 FB	1 1/2	1 1/2 FB	2	2 FB	3
A [in]	14.69	16.1	21.22	21.22	26.3	26.3	30.71	30.71	45.35	45.35
B [in]	0.79	0.79	1.18	1.18	1.1	1.1	1.38	1.38	2.24	2.24
C [in]	1.57	1.57	1.75	1.75	2.36	2.36	3.15	3.15	3.54	3.54


**Zero point adjustment**

All measuring devices are calibrated in accordance with state-of-the-art technology. Calibration takes place under reference conditions (→ 34). Therefore, a zero point adjustment in the field is generally not required.

Experience shows that zero point adjustment is advisable only in special cases:

- To achieve maximum measuring accuracy even with low flow rates
- Under extreme process or operating conditions (e.g. very high process temperatures or very high-viscosity fluids).

### Mounting Safety Barrier Promass 100

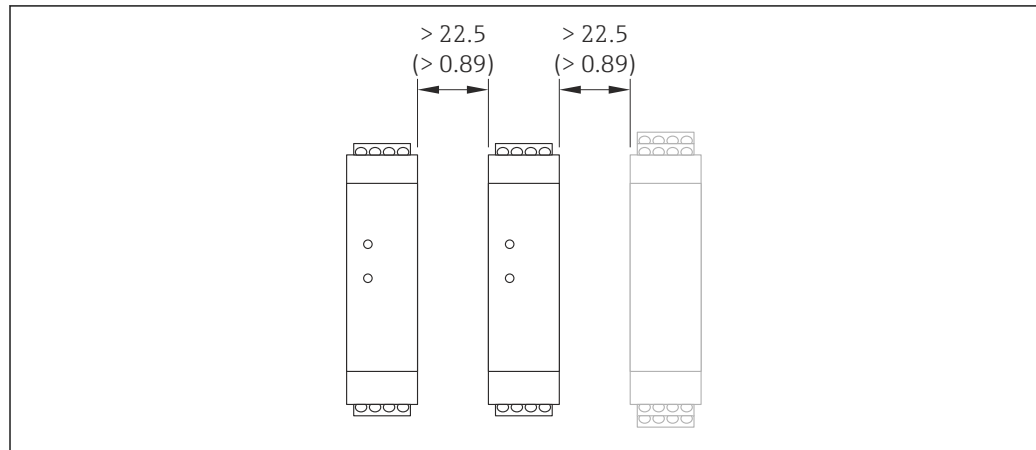

A0016894

- 19 Minimum distance between additional Safety Barrier Promass 100 or other modules. Engineering unit mm (in)

## Environment

### Ambient temperature range

Measuring device	Non-Ex	-40 to +60 °C (-40 to +140 °F)
	Ex na, NI version	-40 to +60 °C (-40 to +140 °F)
	Ex ia, IS version	<ul style="list-style-type: none"> <li>■ -40 to +60 °C (-40 to +140 °F)</li> <li>■ -50 to +60 °C (-58 to +140 °F) (Order code for "Test, certificate", option JM)</li> </ul>
Local display		-20 to +60 °C (-4 to +140 °F) The readability of the display may be impaired at temperatures outside the temperature range.
Safety Barrier Promass 100		-40 to +60 °C (-40 to +140 °F)

- If operating outdoors:  
Avoid direct sunlight, particularly in warm climatic regions.

**i** Weather protection covers can be ordered from Endress+Hauser: see "Accessories" section

### Temperature tables

In the following tables, the following interdependencies between the maximum medium temperature for T1-T6 and the maximum ambient temperature  $T_a$  apply when operating the device in hazardous areas.

#### Ex ia, cCSA<sub>US</sub> IS

SI units

Order code for "Housing"	$T_a$ [°C]	T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
Option A "Compact coated alu"	35	50	85	120	150 <sup>1)</sup>	150 <sup>2)</sup>	150 <sup>2)</sup>
Option B "Compact hygienic, stainless"	50	-	85	120	150 <sup>1)</sup>	150 <sup>2)</sup>	150 <sup>2)</sup>
	60	-	-	120	150 <sup>1)</sup>	150 <sup>2)</sup>	150 <sup>2)</sup>
Option C "Ultra compact hygienic, stainless, M12 device plug"	35	50	85	120	150 <sup>1)</sup>	150 <sup>2)</sup>	150 <sup>2)</sup>

Order code for "Housing"	T <sub>a</sub> [°C]	T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
	45	-	85	120	150 <sup>1)</sup>	150 <sup>2)</sup>	150 <sup>2)</sup>
	50	-	-	120	150 <sup>1)</sup>	150 <sup>2)</sup>	150 <sup>2)</sup>

- 1) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 200 °C: T<sub>m</sub> = 170 °C
- 2) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 200 °C: T<sub>m</sub> = 200 °C

*US units*

Order code for "Housing"	T <sub>a</sub> [°F]	T6 [185 °F]	T5 [212 °F]	T4 [275 °F]	T3 [392 °F]	T2 [572 °F]	T1 [842 °F]
Option A "Compact coated alu"	95	122	185	248	302 <sup>1)</sup>	302 <sup>2)</sup>	302 <sup>2)</sup>
Option B "Compact hygienic, stainless"	122	-	185	248	302 <sup>1)</sup>	302 <sup>2)</sup>	302 <sup>2)</sup>
	140	-	-	248	302 <sup>1)</sup>	302 <sup>2)</sup>	302 <sup>2)</sup>
Option C "Ultra compact hygienic, stainless, M12 device plug"	95	122	185	248	302 <sup>1)</sup>	302 <sup>2)</sup>	302 <sup>2)</sup>
	113	-	185	248	302 <sup>1)</sup>	302 <sup>2)</sup>	302 <sup>2)</sup>
	122	-	-	248	302 <sup>1)</sup>	302 <sup>2)</sup>	302 <sup>2)</sup>

- 1) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 392 °F: T<sub>m</sub> = 338 °F
- 2) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 392 °F: T<sub>m</sub> = 392 °F

**Ex nA, cCSA<sub>US</sub> NI**

*SI units*

Order code for "Housing"	T <sub>a</sub> [°C]	T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
Option A "Compact coated alu"	35	50	85	120	150 <sup>1)</sup>	150 <sup>2)</sup>	150
Option B "Compact hygienic, stainless"	50	-	85	120	150	150	150
	60	-	-	120	150	150	150
Option C "Ultra compact hygienic, stainless, M12 device plug"	50	-	85	120	150	150	150
	60	-	-	120	150	150	150

- 1) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 200 °C: T<sub>m</sub> = 170 °C
- 2) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 200 °C: T<sub>m</sub> = 200 °C

*US units*

Order code for "Housing"	T <sub>a</sub> [°F]	T6 [185 °F]	T5 [212 °F]	T4 [275 °F]	T3 [392 °F]	T2 [572 °F]	T1 [842 °F]
Option A "Compact coated alu"	95	122	185	248	302 <sup>1)</sup>	302 <sup>2)</sup>	302
Option B "Compact hygienic, stainless"	122	-	185	248	302	302	302
	140	-	-	248	302	302	302
Option C "Ultra compact hygienic, stainless, M12 device plug"	122	-	185	248	302	302	302
	140	-	-	248	302	302	302

- 1) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 392 °F: T<sub>m</sub> = 338 °F
- 2) The following applies for specified sensors with a maximum medium temperature T<sub>m</sub> = 392 °F: T<sub>m</sub> = 392 °F

*Explosion hazards arising from gas and dust***Determining the temperature class and surface temperature with the temperature table**

- In the case of gas: Determine the temperature class as a function of the ambient temperature  $T_a$  and the medium temperature  $T_m$ .
- In the case of dust: Determine the maximum surface temperature as a function of the maximum ambient temperature  $T_a$  and the maximum medium temperature  $T_m$ .

**Example**

- Measured maximum ambient temperature:  $T_{ma} = 47\text{ °C}$
- Measured maximum medium temperature:  $T_{mm} = 108\text{ °C}$

	$T_a$ [°C]	$T_6$ [85°C]	$T_5$ [100°C]	$T_4$ [135°C]	$T_3$ [200°C]	$T_2$ [300°C]	$T_1$ [450°C]
	35	50	85	120	140	140	140
	50	-	85	120	140	140	140
	60	-	-	120	140	140	140
	35	50	85	120	140	140	140
	45	-	85	120	140	140	140
	50	-	-	120	140	140	140

Diagram illustrating the procedure for determining the maximum surface temperature. The table shows the relationship between ambient temperature ( $T_a$ ) and medium temperature ( $T_m$ ) and the resulting temperature class ( $T_1$  to  $T_6$ ). The measured maximum ambient temperature ( $T_{ma} = 47\text{ °C}$ ) is used to select the appropriate  $T_a$  value (50°C). The measured maximum medium temperature ( $T_{mm} = 108\text{ °C}$ ) is used to select the appropriate  $T_m$  value (50°C). The intersection of these values in the table indicates the temperature class  $T_4$  (135°C).

**20 Procedure for determining the maximum surface temperature**

1. Select device.
2. In the column for the maximum ambient temperature  $T_a$  select the temperature that is immediately greater than or equal to the measured maximum ambient temperature  $T_{ma}$  that is present.
  - ↳  $T_a = 50\text{ °C}$ .
  - The row showing the maximum medium temperature is determined.
3. Select the maximum medium temperature  $T_m$  of this row, which is larger or equal to the measured maximum medium temperature  $T_{mm}$ .
  - ↳ The column with the temperature class for gas is determined:  $108\text{ °C} \leq 120\text{ °C} \rightarrow T_4$ .
4. The maximum temperature of the temperature class determined corresponds to the maximum surface temperature for dust:  $T_4 = 135\text{ °C}$

**Storage temperature** -50 to +60 °C (-58 to +140 °F) (Order code for "Test, certificate", option JM)

**Climate class** DIN EN 60068-2-38 (test Z/AD)

**Degree of protection****Transmitter and sensor**

- As standard: IP66/67, type 4X enclosure
- With the order code for "Sensor options", option **CM**: IP69K can also be ordered
- When housing is open: IP20, type 1 enclosure
- Display module: IP20, type 1 enclosure

**Safety Barrier Promass 100**

IP20

**Shock resistance** As per IEC/EN 60068-2-31


**Vibration resistance** Acceleration up to 1 g, 10 to 150 Hz, based on IEC/EN 60068-2-6

**Interior cleaning**

- Sterilization in place (SIP)
- Cleaning in place (CIP)
- Cleaning with pigs

**Electromagnetic compatibility (EMC)**

- As per IEC/EN 61326 and NAMUR Recommendation 21 (NE 21)
- Complies with emission limits for industry as per EN 55011 (Class A)
- Device version with PROFIBUS DP: Complies with emission limits for industry as per EN 50170 Volume 2, IEC 61784

 The following applies for PROFIBUS DP: If baud rates > 1.5 MBaud an EMC cable entry must be used and the cable shield must continue as far as the terminal wherever possible.

 For details refer to the Declaration of Conformity.

## Process

**Medium temperature range**

**Sensor**  
-50 to +150 °C (-58 to +302 °F)

**Seals**  
No internal seals


**Density**


0 to 5 000 kg/m<sup>3</sup> (0 to 312 lb/cf)

**Pressure-temperature ratings**

The following pressure-temperature ratings refer to the entire device and not just the process connection.


**Flange connection according to EN 1092-1 (DIN 2501)**

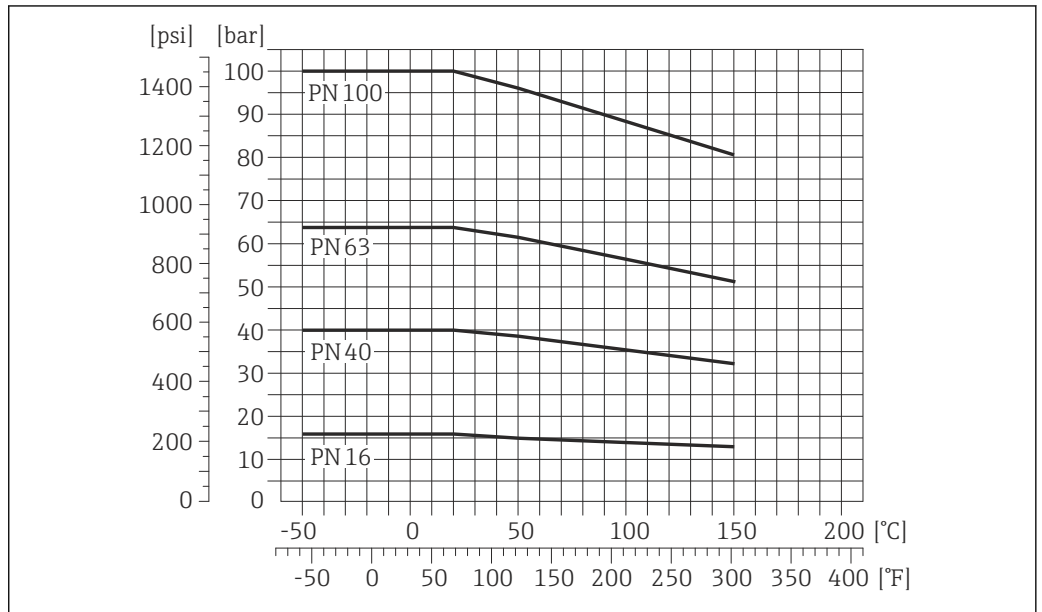

 21 With flange material 1.4301 (304); wetted parts: titanium

A0020873-EN


Flange connection according to ASME B16.5

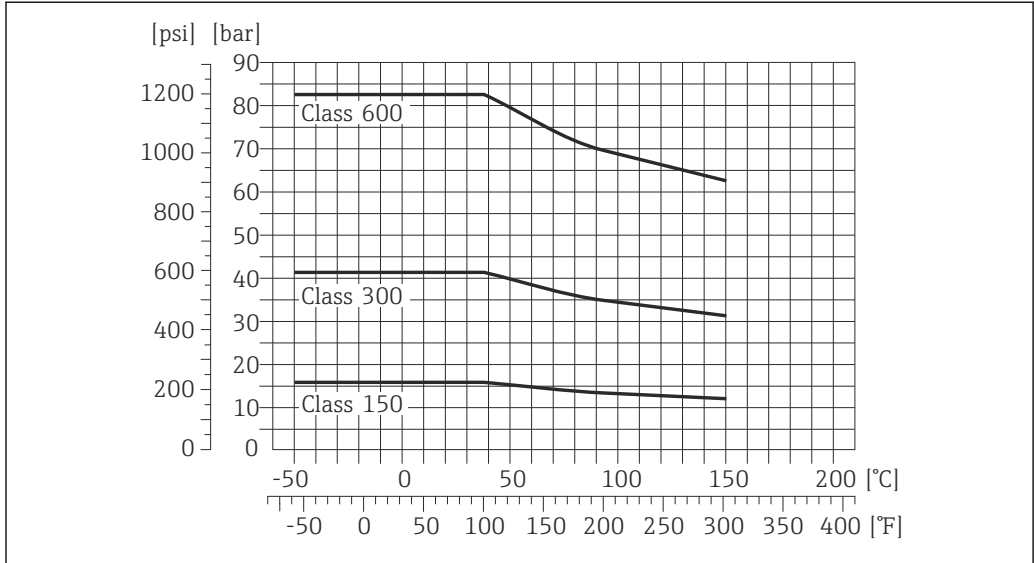

A0020923-EN

22 With flange material 1.4301 (304); wetted parts: titanium


Flange connection according to JIS B2220

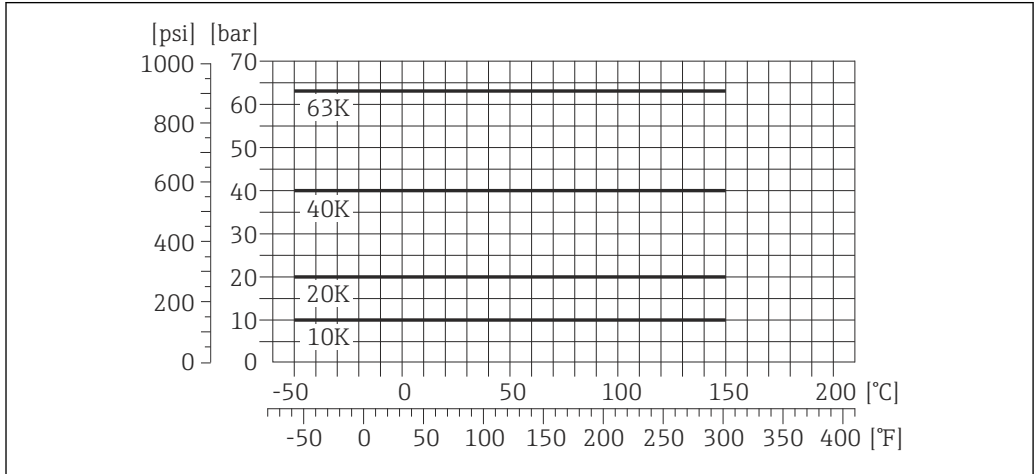

A0020924-EN

23 With flange material 1.4301 (304). Wetted parts: titanium.

**Process connection to DIN 11851**

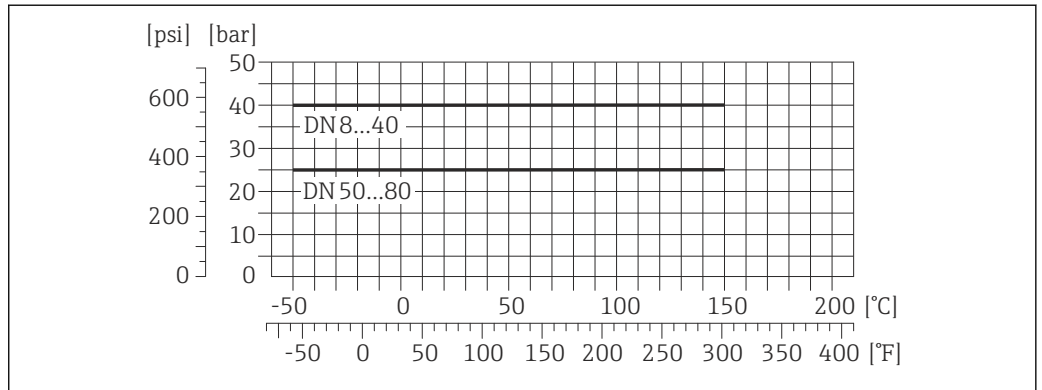


A0021004-EN

24 With titanium connection material

DIN 11851 allows for applications up to +140 °C (+284 °F) if suitable sealing materials are used. Please take this into account when selecting seals and counterparts, as these components can limit the pressure and temperature range.


**Aseptic threaded adapter as per DIN 11864-1 Form A**

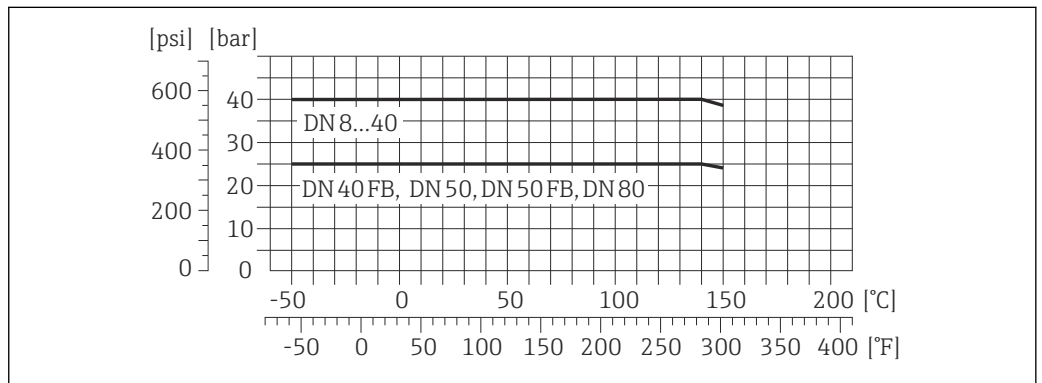

A0020925-EN

25 With titanium connection material


**Aseptic flange connection according to DIN 11864-2 Form A**

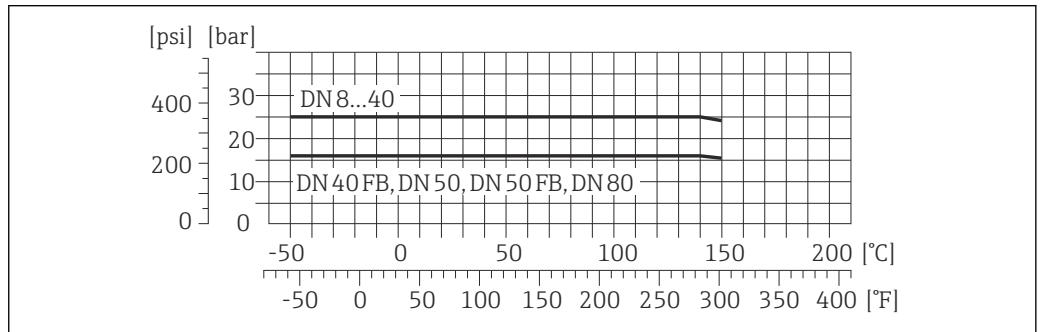

A0020926-EN

26 With titanium flange material

## Threaded hygienic connection to ISO 2853

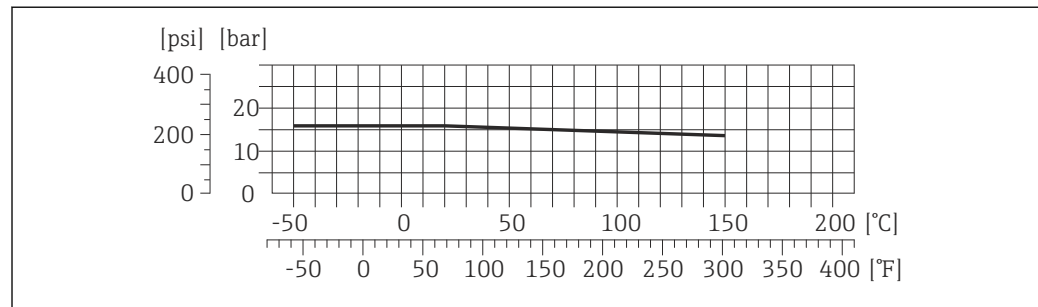

A0020919-EN

27 With titanium connection material

## Tri-Clamp

The clamp connections are suitable up to a maximum pressure of 16 bar (232 psi). Please observe the operating limits of the clamp and seal used as they could be under 16 bar (232 psi). The clamp and seal are not included in the scope of supply.

## Secondary containment pressure rating

The sensor housing is filled with dry nitrogen and protects the electronics and mechanics inside.

DN		Secondary containment nominal pressure (designed with a safety factor $\geq 4$ )		Secondary containment burst pressure	
[mm]	[in]	[bar]	[psi]	[bar]	[psi]
8	$\frac{3}{8}$	40	580	220	3190
15	$\frac{1}{2}$	40	580	220	3190
15 FB	$\frac{1}{2}$ FB	40	580	235	3405
25	1	40	580	235	3405
25 FB	1 FB	40	580	220	3190
40	$1\frac{1}{2}$	40	580	220	3190
40 FB	$1\frac{1}{2}$ FB	40	580	235	3405
50	2	40	580	235	3405
50 FB	2 FB	40	580	460	6670
80	3	40	580	460	6670

FB = Full bore

**i** If there is a risk of measuring tube failure due to process characteristics, e.g. with corrosive process fluids, we recommend the use of sensors whose secondary containment is equipped with special pressure monitoring connections (order code for "Purge connection", option CH).

With the help of these connections, the fluid collected in the secondary containment can be bled off in the event of tube failure. This is especially important in high-pressure gas applications. These connections can also be used for gas purging (gas detection).

Do not open the purge connections unless the containment can be filled immediately with a dry, inert gas. Use only low gauge pressure to purge. Maximum pressure: 5 bar (72.5 psi).

If a device fitted with purge connections is connected to the purge system, the maximum nominal pressure is determined by the purge system itself or by the device, depending on which component has the lower nominal pressure.

Dimensions: (→ 71)

## Flow limit

Select the nominal diameter by optimizing between the required flow range and permissible pressure loss.



**i** For an overview of the measuring range full scale values, see the "Measuring range" section (→ 8)

- The minimum recommended full scale value is approx. 1/20 of the maximum full scale value
- In most applications, 20 to 50 % of the maximum full scale value can be considered ideal
- Select a lower full scale value for abrasive substances (such as liquids with entrained solids): flow velocity < 1 m/s (< 3 ft/s).
- For gas measurement the following rules apply:
  - The flow velocity in the measuring tubes should not exceed half the sonic velocity (0.5 Mach).
  - The maximum mass flow depends on the density of the gas: formula (→ 8)

**Pressure loss**


**i** To calculate the pressure loss, use the *Applicator* sizing tool (→ 82)

**System pressure**

It is important that cavitation does not occur, or that gases entrained in the liquids do not outgas. This is prevented by means of a sufficiently high system pressure.

For this reason, the following mounting locations are recommended:


- At the lowest point in a vertical pipe
- Downstream from pumps (no danger of vacuum)

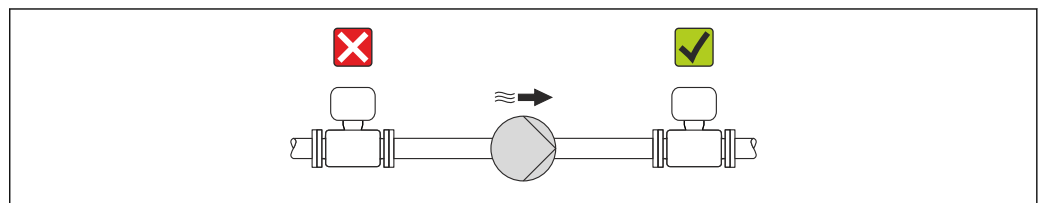

A0015594

**Thermal insulation**

In the case of some fluids, it is important that the heat radiated from the sensor to the transmitter is kept to a minimum. A wide range of materials can be used for the required insulation.

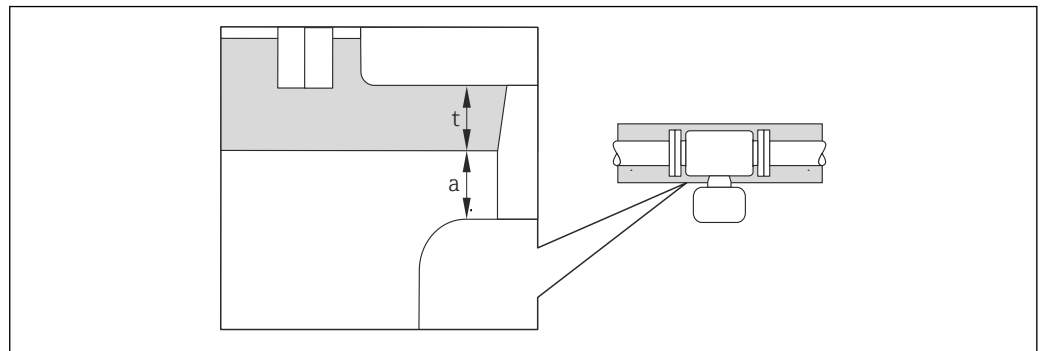


A0019919

*a* Minimum distance to insulation

*t* Insulation thickness

The minimum distance between the transmitter housing and the insulation is 10 mm (0.39 in) so that the transmitter head remains completely exposed.


**Insulation thickness for version without neck extension**

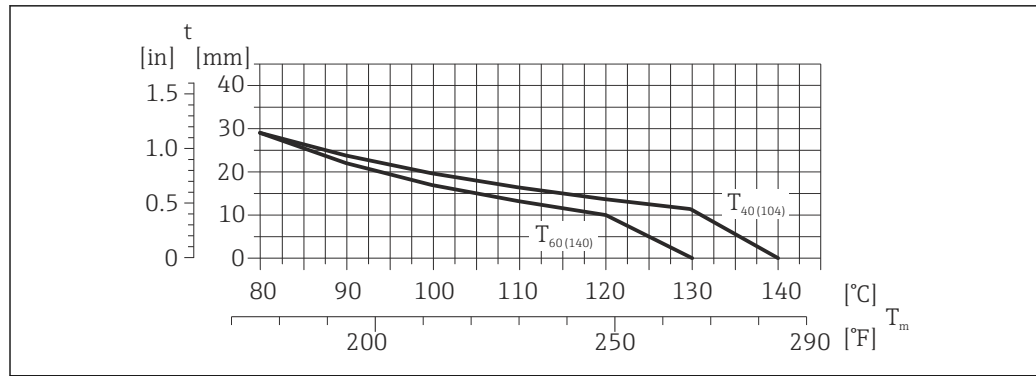

A0023173

28 Recommended insulation thicknesses depending on the medium and ambient temperature

$t$	Insulation thickness
$T_m$	Medium temperature
$T_{40(104)}$	Insulation thickness with ambient temperature of $T_a = 40\text{ °C}$ ( $104\text{ °F}$ )
$T_{60(140)}$	Insulation thickness with ambient temperature of $T_a = 60\text{ °C}$ ( $140\text{ °F}$ )

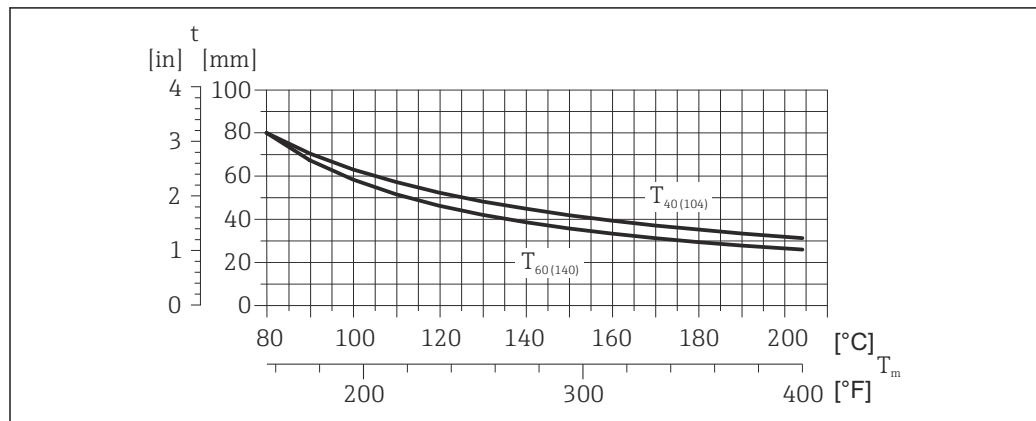

A0023177

29 Recommended insulation thicknesses depending on the medium and ambient temperature

$t$	Insulation thickness
$T_m$	Medium temperature
$T_{40(104)}$	Insulation thickness with ambient temperature of $T_a = 40\text{ °C}$ ( $104\text{ °F}$ )
$T_{60(140)}$	Insulation thickness with ambient temperature of $T_a = 60\text{ °C}$ ( $140\text{ °F}$ )

#### NOTICE

**The insulation can also be thicker than the recommended insulation thickness.**

Prerequisite:

- ▶ The temperature at the lower end of the transmitter housing does not exceed  $80\text{ °C}$  ( $176\text{ °F}$ )
- ▶ Ensure that convection takes place on a sufficiently large scale at the transmitter neck.
- ▶ Ensure that a sufficiently large area of the housing support remains exposed. The uncovered part serves as a radiator and protects the electronics from overheating and excessive cooling.

## Heating

Some fluids require suitable measures to avoid loss of heat at the sensor.

### Heating options

- Electrical heating, e.g. with electric band heaters
- Via pipes carrying hot water or steam
- Via heating jackets



Heating jackets for the sensor can be ordered as accessories from Endress+Hauser (→ 81).

**Vibrations**


The high oscillation frequency of the measuring tubes ensures that the correct operation of the measuring system is not influenced by plant vibrations.

## Mechanical construction

### Design, dimensions

#### Compact version

Order code for "Housing", option A "Compact coated alu"

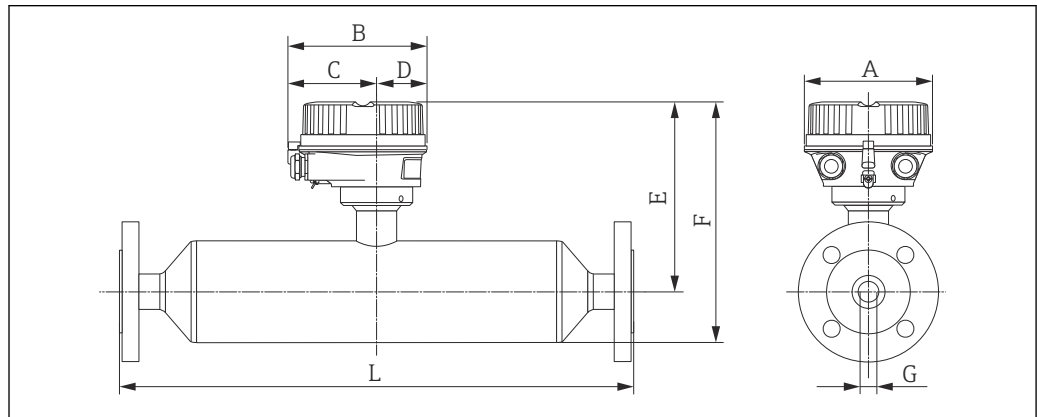

A0016456

#### Dimensions SI units

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E <sup>1) 2)</sup> [mm]	F <sup>1) 2)</sup> [mm]	G [mm]	L [mm]
8	136	147.5	93.5	54	207.2	264.4	8.55	<sup>3)</sup>
15	136	147.5	93.5	54	207.2	264.4	11.38	<sup>3)</sup>
15 FB	136	147.5	93.5	54	207.2	264.4	17.07	<sup>3)</sup>
25	136	147.5	93.5	54	216.9	274.1	17.07	<sup>3)</sup>
25 FB	136	147.5	93.5	54	216.9	287.6	26.40	<sup>3)</sup>
40	136	147.5	93.5	54	231.2	301.9	26.40	<sup>3)</sup>
40 FB	136	147.5	93.5	54	231.2	315.4	35.62	<sup>3)</sup>
50	136	147.5	93.5	54	256.6	340.8	35.62	<sup>3)</sup>
50 FB	136	147.5	93.5	54	256.6	366.2	54.8	<sup>3)</sup>
80	136	147.5	93.5	54	256.6	366.2	54.8	<sup>3)</sup>

FB = Full bore

- 1) If using an extension neck for the extended temperature range, order code for "Sensor option", option CG: values +70 mm
- 2) If using a display, order code for "Display; Operation", option B: values +28 mm
- 3) dependent on respective process connection

#### Dimensions US units


DN [in]	A [in]	B [in]	C [in]	D [in]	E <sup>2)</sup> [in]	F <sup>1) 2)</sup> [in]	G [in]	L [in]
$\frac{3}{8}$	5.35	5.81	3.68	2.13	8.16	10.41	0.34	<sup>3)</sup>
$\frac{1}{2}$	5.35	5.81	3.68	2.13	8.16	10.41	0.45	<sup>3)</sup>
$\frac{1}{2}$ FB	5.35	5.81	3.68	2.13	8.16	10.41	0.67	<sup>3)</sup>
1	5.35	5.81	3.68	2.13	8.54	10.79	0.67	<sup>3)</sup>
1 FB	5.35	5.81	3.68	2.13	8.54	11.32	1.01	<sup>3)</sup>
1½	5.35	5.81	3.68	2.13	9.1	11.89	1.01	<sup>3)</sup>
1½ FB	5.35	5.81	3.68	2.13	9.1	12.42	1.40	<sup>3)</sup>

DN [in]	A [in]	B [in]	C [in]	D [in]	E <sup>2)</sup> [in]	F <sup>1) 2)</sup> [in]	G [in]	L [in]
2	5.35	5.81	3.68	2.13	10.1	13.42	1.40	<sup>3)</sup>
2FB	5.35	5.81	3.68	2.13	10.1	14.42	2.16	<sup>3)</sup>
3	5.35	5.81	3.68	2.13	10.1	14.42	2.16	<sup>3)</sup>

FB = Full bore

- 1) If using an extension neck for the extended temperature range, order code for "Sensor option", option CG: values +2.76 in
- 2) If using a display, order code for "Display; Operation", option B: values +1.1 in
- 3) dependent on respective process connection

Order code for "Housing", option B "Compact hygienic, stainless"

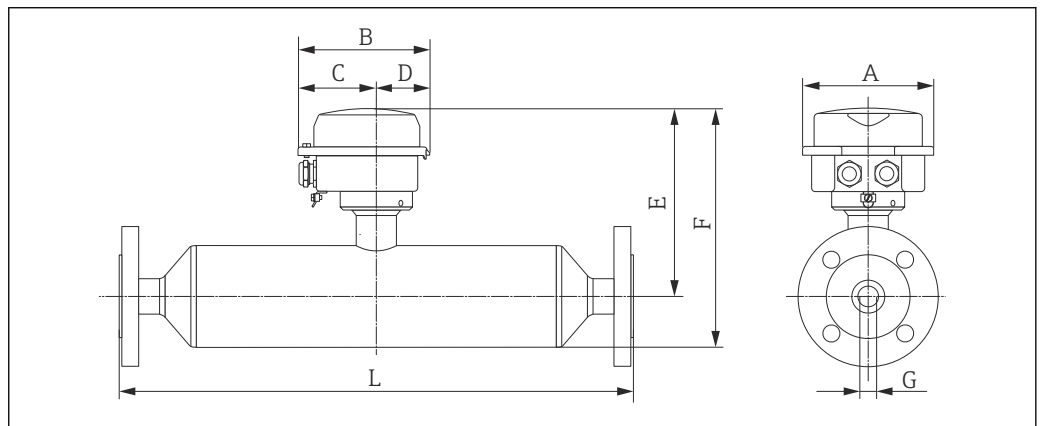

A0016522

Dimensions SI units

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E <sup>2)</sup> [mm]	F <sup>1) 2)</sup> [mm]	G [mm]	L [mm]
8	133.5	136.8	78	58.8	202.2	264.4	8.55	<sup>3)</sup>
15	133.5	136.8	78	58.8	202.2	264.4	11.38	<sup>3)</sup>
15 FB	133.5	136.8	78	58.8	202.2	264.4	17.07	<sup>3)</sup>
25	133.5	136.8	78	58.8	211.9	274.1	17.07	<sup>3)</sup>
25 FB	133.5	136.8	78	58.8	211.9	287.6	26.40	<sup>3)</sup>
40	133.5	136.8	78	58.8	226.2	301.9	26.40	<sup>3)</sup>
40 FB	133.5	136.8	78	58.8	226.2	315.4	35.62	<sup>3)</sup>
50	133.5	136.8	78	58.8	251.6	340.8	35.62	<sup>3)</sup>
50 FB	133.5	136.8	78	58.8	251.6	366.2	54.8	<sup>3)</sup>
80	133.5	136.8	78	58.8	251.6	366.2	54.8	<sup>3)</sup>

FB = Full bore

- 1) If using an extension neck for the extended temperature range, order code for "Sensor option", option CG: values +70 mm
- 2) If using a display, order code for "Display; Operation", option B: values +14 mm
- 3) dependent on respective process connection


## Dimensions US units

DN [in]	A [in]	B [in]	C [in]	D [in]	E <sup>2)</sup> [in]	F <sup>1) 2)</sup> [in]	G [in]	L [in]
3/8	5.26	5.39	3.07	2.31	7.96	10.41	0.34	<sup>3)</sup>
1/2	5.26	5.39	3.07	2.31	7.96	10.41	0.45	<sup>3)</sup>
1/2 FB	5.26	5.39	3.07	2.31	7.96	10.41	0.67	<sup>3)</sup>
1	5.26	5.39	3.07	2.31	8.34	10.79	0.67	<sup>3)</sup>
1 FB	5.26	5.39	3.07	2.31	8.34	11.32	1.01	<sup>3)</sup>
1 1/2	5.26	5.39	3.07	2.31	8.91	11.89	1.01	<sup>3)</sup>
1 1/2 FB	5.26	5.39	3.07	2.31	8.91	12.42	1.40	<sup>3)</sup>
2	5.26	5.39	3.07	2.31	9.91	13.42	1.40	<sup>3)</sup>
2 FB	5.26	5.39	3.07	2.31	9.91	14.42	2.16	<sup>3)</sup>
3	5.26	5.39	3.07	2.31	9.91	14.42	2.16	<sup>3)</sup>

FB = Full bore

- 1) If using an extension neck for the extended temperature range, order code for "Sensor option", option CG: values +2.76 in
- 2) If using a display, order code for "Display; Operation", option B: values +0.55 in
- 3) dependent on respective process connection

Order code for "Housing", option C "Ultra compact hygienic, stainless, M12 device plug"

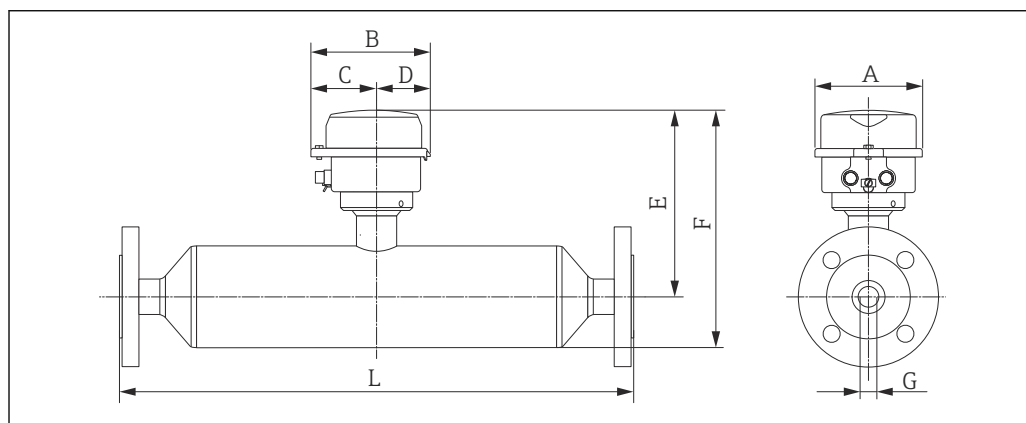

A0016521

## Dimensions SI units

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E <sup>2)</sup> [mm]	F <sup>1) 2)</sup> [mm]	G [mm]	L [mm]
8	111.4	123.6	67.7	55.9	202.2	264.4	8.56	<sup>3)</sup>
15	111.4	123.6	67.7	55.9	202.2	264.4	11.38	<sup>3)</sup>
15 FB	111.4	123.6	67.7	55.9	202.2	264.4	17.07	<sup>3)</sup>
25	111.4	123.6	67.7	55.9	211.9	274.1	17.07	<sup>3)</sup>
25 FB	111.4	123.6	67.7	55.9	211.9	287.6	26.37	<sup>3)</sup>
40	111.4	123.6	67.7	55.9	226.2	301.9	26.37	<sup>3)</sup>
40 FB	111.4	123.6	67.7	55.9	226.2	315.4	35.62	<sup>3)</sup>
50	111.4	123.6	67.7	55.9	251.6	340.8	35.62	<sup>3)</sup>
50 FB	111.4	123.6	67.7	55.9	251.6	366.2	54.76	<sup>3)</sup>

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E <sup>2)</sup> [mm]	F <sup>1) 2)</sup> [mm]	G [mm]	L [mm]
80	111.4	123.6	67.7	55.9	251.6	366.2	54.76	<sup>3)</sup>
FB = Full bore								

- 1) If using an extension neck for the extended temperature range, order code for "Sensor option", option CG: values +70 mm
- 2) If using a display, order code for "Display; Operation", option B: values +14 mm
- 3) dependent on respective process connection


*Dimensions US units*

DN [in]	A [in]	B [in]	C [in]	D [in]	E <sup>2)</sup> [in]	F <sup>1) 2)</sup> [in]	G [in]	L [in]
$\frac{3}{8}$	4.39	4.87	2.67	2.2	7.96	10.41	0.337	<sup>3)</sup>
$\frac{1}{2}$	4.39	4.87	2.67	2.2	7.96	10.41	0.448	<sup>3)</sup>
$\frac{1}{2}$ FB	4.39	4.87	2.67	2.2	7.96	10.41	0.672	<sup>3)</sup>
1	4.39	4.87	2.67	2.2	8.34	10.79	0.672	<sup>3)</sup>
1 FB	4.39	4.87	2.67	2.2	8.34	11.32	1.038	<sup>3)</sup>
$1\frac{1}{2}$	4.39	4.87	2.67	2.2	8.91	11.89	1.038	<sup>3)</sup>
$1\frac{1}{2}$ FB	4.39	4.87	2.67	2.2	8.91	12.42	1.402	<sup>3)</sup>
2	4.39	4.87	2.67	2.2	9.91	13.42	1.402	<sup>3)</sup>
2 FB	4.39	4.87	2.67	2.2	9.91	14.42	2.156	<sup>3)</sup>
3	4.39	4.87	2.67	2.2	9.91	14.42	2.156	<sup>3)</sup>
FB = Full bore								

- 1) If using an extension neck for the extended temperature range, order code for "Sensor option", option CG: values +2.76 in
- 2) If using a display, order code for "Display; Operation", option B: values +0.55 in
- 3) dependent on respective process connection

**Process connections in SI units**

*Flange connections EN (DIN)*

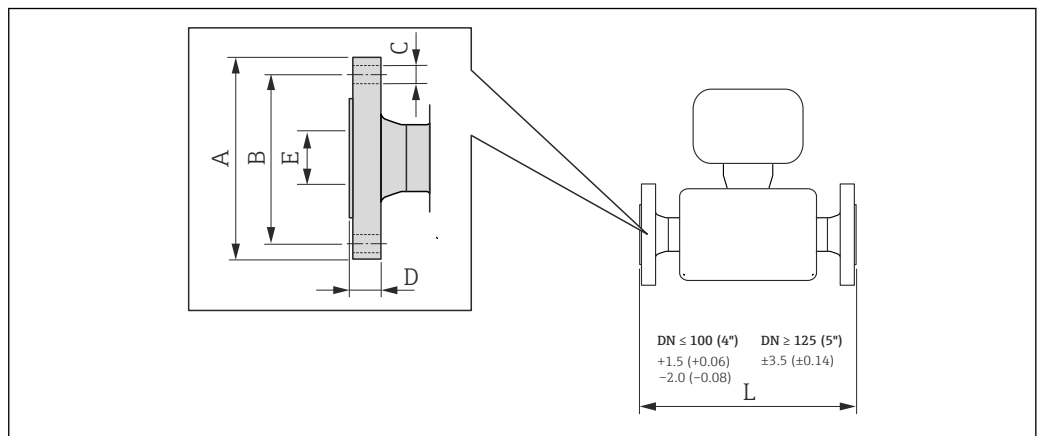

30 Engineering unit mm (in)

A0015621

Flange according to EN 1092-1 (DIN 2501), PN 40: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option D2W)						
Surface roughness (flange): EN 1092-1 Form B1 (DIN 2526 Form C), Ra 3.2 to 12.5 µm						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	95	65	4 × Ø14	16	17.30	402
15	95	65	4 × Ø14	16	17.30	438
15 FB	95	65	4 × Ø14	15	17.07	572
25	115	85	4 × Ø14	19	28.50	578
25 FB	115	85	4 × Ø14	18	25.60	700
40	150	110	4 × Ø18	22	43.10	708
40 FB	150	110	4 × Ø18	20	35.62	819
50	165	125	4 × Ø18	24	54.50	827
50 FB	165	125	4 × Ø18	36	54.8	1210
80	200	160	8 × Ø18	33	82.5	1210
FB = Full bore						

1) DN 8 with DN 15 flanges as standard


Flange according to EN 1092-1 (DIN 2501), PN 63: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option D3W)						
Surface roughness (flange): EN 1092-1 Form B2 (DIN 2526 Form E), Ra 0.8 to 3.2 µm						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
50	180	135	4 × Ø22	34	54.5	832
50FB	180	135	4 × Ø22	45	54.8	1210
80	215	170	8 × Ø22	41	81.7	1210
FB = Full bore						

Flange according to EN 1092-1 (DIN 2501 / DIN 2512N), PN 100: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option D4W)						
Surface roughness (flange): EN 1092-1 Form B2 (DIN 2526 Form E), Ra 0.8 to 3.2 µm						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	105	75	4 × Ø14	25	17.30	402
15	105	75	4 × Ø14	25	17.30	438
15 FB	105	75	4 × Ø14	26	17.07	578
25	140	100	4 × Ø18	29	28.50	578
25 FB	140	100	4 × Ø18	31	25.60	706
40	170	125	4 × Ø22	32	42.50	708
40 FB	170	125	4 × Ø22	33	35.62	825
50	195	145	4 × Ø26	36	53.90	832
50 FB	195	145	4 × Ø26	48	54.8	1210
80	230	180	8 × Ø26	58	80.9	1236
FB = Full bore						

1) DN 8 with DN 15 flanges as standard



Flange connections ASME B16.5

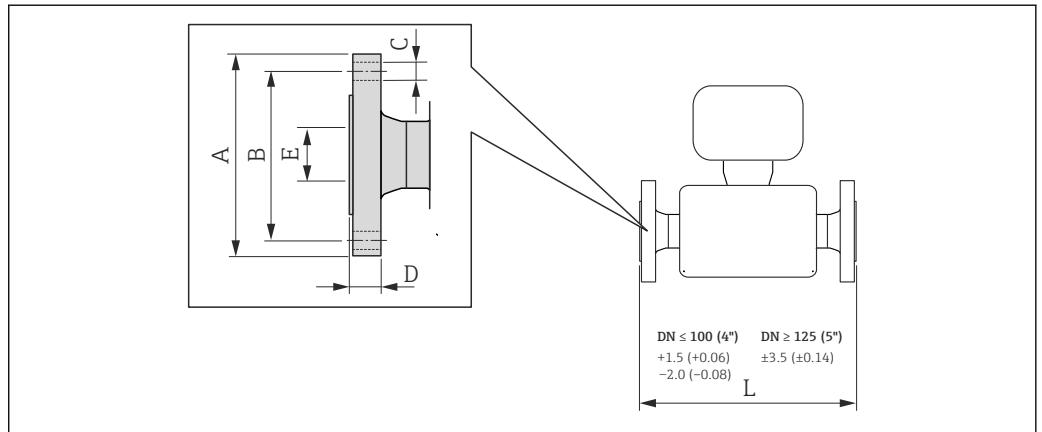

A0015621

31 Engineering unit mm (in)

**Flange according to ASME B16.5, Cl 150: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option AAW)**

Surface roughness (flange): Ra 3.2 to 6.3 µm

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	90	60.3	4 × Ø15.7	20	15.70	402
15	90	60.3	4 × Ø15.7	20	15.70	438
15 FB	90	60.3	4 × Ø15.7	19	17.07	572
25	110	79.4	4 × Ø15.7	23	26.70	578
25 FB	110	79.4	4 × Ø15.7	22	25.60	700
40	125	98.4	4 × Ø15.7	26	40.90	708
40 FB	125	98.4	4 × Ø15.7	24	35.62	819
50	150	120.7	4 × Ø19.1	28	52.60	827
50 FB	150	120.7	4 × Ø19.1	40	54.8	1210
80	190	152.4	4 × Ø19.1	37	78	1210

FB = Full bore

1) DN 8 with DN 15 flanges as standard

**Flange according to ASME B16.5, Cl 300: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option ABW)**

Surface roughness (flange): Ra 3.2 to 6.3 µm

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	95	66.7	4 × Ø15.7	20	15.70	402
15	95	66.7	4 × Ø15.7	20	15.70	438
15 FB	95	66.7	4 × Ø15.7	19	17.07	572
25	125	88.9	4 × Ø19.1	23	26.70	578
25 FB	125	88.9	4 × Ø19.1	22	25.60	700
40	155	114.3	4 × Ø22.4	26	40.90	708
40 FB	155	114.3	4 × Ø22.4	24	35.62	819

Flange according to ASME B16.5, Cl 300: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option ABW)						
Surface roughness (flange): Ra 3.2 to 6.3 $\mu\text{m}$						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
50	165	127.0	8 × Ø19.1	28	52.60	827
50 FB	165	127.0	8 × Ø19.1	43	54.8	1210
80	210	168.3	8 × Ø22.3	42	78	1210

FB = Full bore


1) DN 8 with DN 15 flanges as standard

Flange according to ASME B16.5, Cl 600: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option ACW)						
Surface roughness (flange): Ra 3.2 to 6.3 $\mu\text{m}$						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	95	66.7	4 × Ø15.7	20	13.80	402
15	95	66.7	4 × Ø15.7	20	13.80	438
15 FB	95	66.7	4 × Ø15.7	22	17.07	578
25	125	88.9	4 × Ø19.1	23	24.40	578
25 FB	125	88.9	4 × Ø19.1	25	25.60	706
40	155	114.3	4 × Ø22.4	28	38.10	708
40 FB	155	114.3	4 × Ø22.4	29	35.62	825
50	165	127.0	8 × Ø19.1	33	49.30	832
50 FB	165	127.0	8 × Ø19.1	46	54.8	1210
80	210	168.3	8 × Ø22.3	53	73.7	1222

FB = Full bore

1) DN 8 with DN 15 flanges as standard

### Flange connections JIS

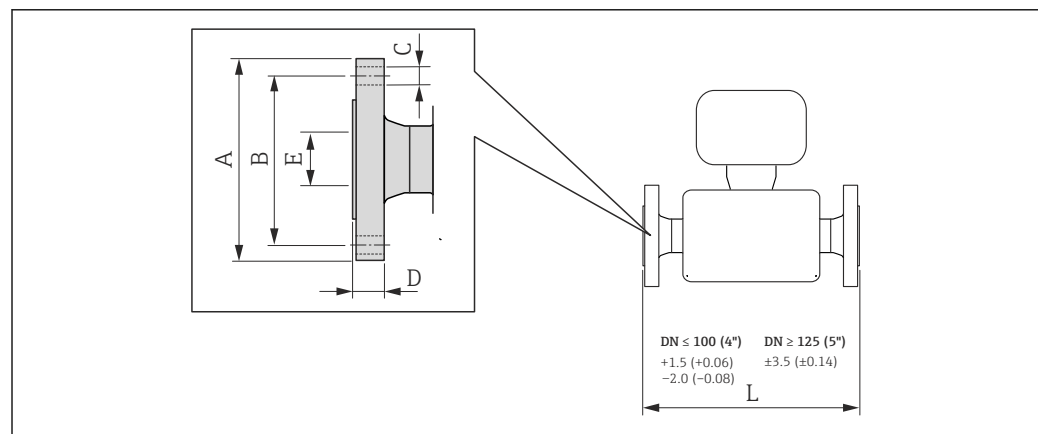

A0015621

32 Engineering unit mm (in)

**Flange JIS B2220, 10K: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option NDW)**

Surface roughness (flange): Ra 3.2 to 6.3 µm

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
50	155	120	4 × Ø19	28	50	827
50 FB	195	145	4 × Ø26	48	54.8	1210
80	200	160	8 × Ø18	37	82.5	1210

FB = Full bore

**Flange JIS B2220, 20K: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option NEW)**

Surface roughness (flange): Ra 3.2 to 6.3 µm

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	95	70	4 × Ø15	20	15.00	402
15	95	70	4 × Ø15	20	15.00	438
15 FB	95	70	4 × Ø15	19	17.07	572
25	125	90	4 × Ø19	23	25.00	578
25 FB	125	90	4 × Ø19	22	25.60	700
40	140	105	4 × Ø19	26	40.00	708
40 FB	140	105	4 × Ø19	24	35.62	819
50	155	120	8 × Ø19	28	50.00	827
50 FB	155	120	8 × Ø19	42	54.8	1210
80	200	160	8 × Ø23	36	80	1210

FB = Full bore

1) DN 8 with DN 15 flanges as standard

**Flange JIS B2220, 40K: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option NFW)**

Surface roughness (flange): Ra 3.2 to 6.3 µm

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	115	80	4 × Ø19	25	15.00	402
15	115	80	4 × Ø19	25	15.00	438
15 FB	115	80	4 × Ø19	26	17.07	578
25	130	95	4 × Ø19	27	25.00	578
25 FB	130	95	4 × Ø19	29	25.60	706
40	160	120	4 × Ø23	30	38.00	708
40 FB	160	120	4 × Ø23	31	35.62	825
50	165	130	8 × Ø19	32	50.00	827
50 FB	165	130	8 × Ø19	43	54.8	1210
80	210	170	8 × Ø23	46	75	1210

FB = Full bore


1) DN 8 with DN 15 flanges as standard

Flange JIS B2220, 63K: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option NHW)						
Surface roughness (flange): Ra 3.2 to 6.3 µm						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	120	85	4 × Ø19	28	12.00	402
15	120	85	4 × Ø19	28	12.80	438
15 FB	120	85	4 × Ø19	29	17.07	578
25	140	100	4 × Ø23	30	22.00	578
25 FB	140	100	4 × Ø23	32	25.60	706
40	175	130	4 × Ø25	36	35.00	708
40 FB	175	130	4 × Ø25	37	35.62	825
50	185	145	8 × Ø23	40	48.00	832
50 FB	185	145	8 × Ø23	47	54.8	1210
80	230	185	8 × Ø25	55	73	1226

FB = Full bore

1) DN 8 with DN 15 flanges as standard

### Tri-Clamp

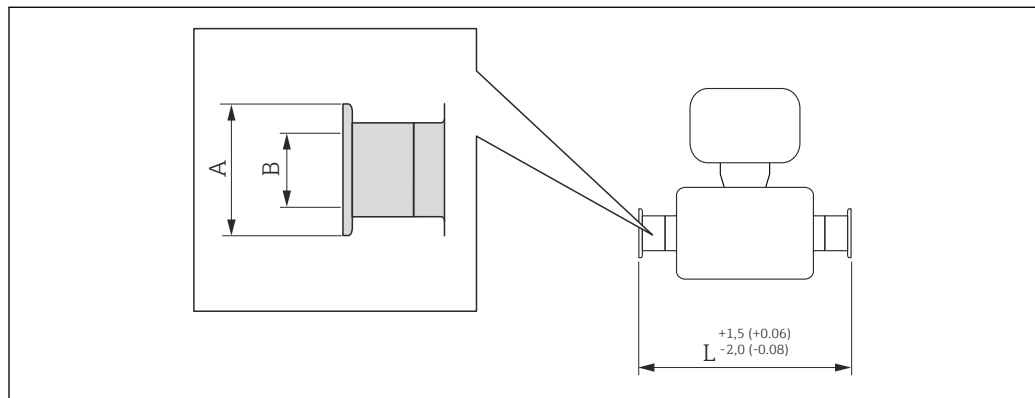

A0015625

33 Engineering unit mm (in)

1", 1½", 2" -Tri-Clamp for pipe size: titanium (order code for "Process connection", option FTW)				
DN [mm]	Clamp [in]	A [mm]	B [mm]	L [mm]
8	1	50.4	22.1	427
15	1	50.4	22.1	463
15 FB	see ¾" Tri-Clamp connection			
25	1	50.4	22.1	603
25 FB	1	50.4	22.1	730
40	1½	50.4	34.8	731
40 FB	1½	50.4	34.8	849
50	2	63.9	47.5	850
50 FB <sup>1)</sup>	2½	77.4	60.3	1268

1", 1½", 2" - Tri-Clamp for pipe size: titanium (order code for "Process connection", option FTW)				
DN [mm]	Clamp [in]	A [mm]	B [mm]	L [mm]
80	3	90.9	72.9	1268

3A version available (order code for "Additional approval", option LP) in combination with  $Ra \leq 0.8 \mu\text{m}$ ,  $Ra \leq 0.4 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)  
 FB = Full bore

1) Order code for "Process connection", option FRW


¾" Tri-Clamp: titanium (order code for "Process connection", option FEW)				
DN [mm]	Clamp [in]	A [mm]	B [mm]	L [mm]
8	¾	25.0	16.0	426
15	¾	25.0	16.0	462
15 FB	¾	25.0	16.0	602

3A version available (order code for "Additional approval", option LP) in combination with  $Ra \leq 0.8 \mu\text{m}$ ,  $Ra \leq 0.4 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)  
 FB = Full bore

½" Tri-Clamp: titanium (order code for "Process connection", option FBW)				
DN [mm]	Clamp [in]	A [mm]	B [mm]	L [mm]
8	½	25.0	9.5	426
15	½	25.0	9.5	462

3A version available (order code for "Additional approval", option LP) in combination with  $Ra \leq 0.8 \mu\text{m}$ ,  $Ra \leq 0.4 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)

*Eccentric Tri-Clamp*

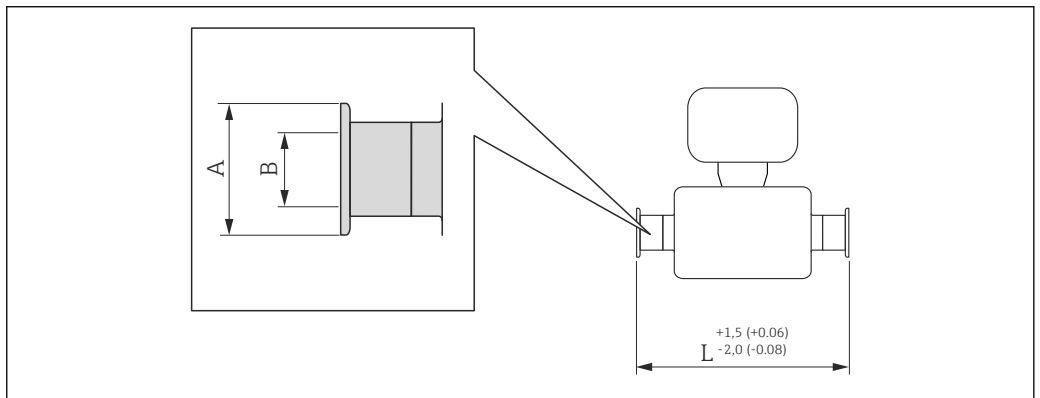


34 Engineering unit mm (in)

Eccentric Tri-Clamp: Titanium					
DN [mm]	Order code for "Process connection", Option	Clamp [in]	A [mm]	B [mm]	L [mm]
8	FEA	½	25	9.5	427
15	FEC	¾	25	15.75	463

Eccentric Tri-Clamp: Titanium					
DN [mm]	Order code for "Process connection", Option	Clamp [in]	A [mm]	B [mm]	L [mm]
15 FB	FEE	1	50.5	22.1	603
25	FEE	1	50.5	22.1	603
25 FB	FEG	1½	50.5	34.8	730
40	FEG	1½	50.5	34.8	730
40 FB	FEJ	2	64	47.5	849
50	FEJ	2	64	47.5	849
50 FB	FEL	2 ½	77.5	60.3	1268
50 FB	FEM	3	91	72.9	1268
80	FEL	2 ½	77.5	60.3	1268
80	FEM	3	91	72.9	1268

3A version available (order code for "Additional approval", option LP) in combination with  $R_a \leq 0.8 \mu\text{m}$ ,  $R_a \leq 0.4 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)  
 FB = Full bore  
 Additional information on "Eccentric clamps ( $\rightarrow$  40)

*Threaded hygienic connection DIN 11851 (sanitary connection)*

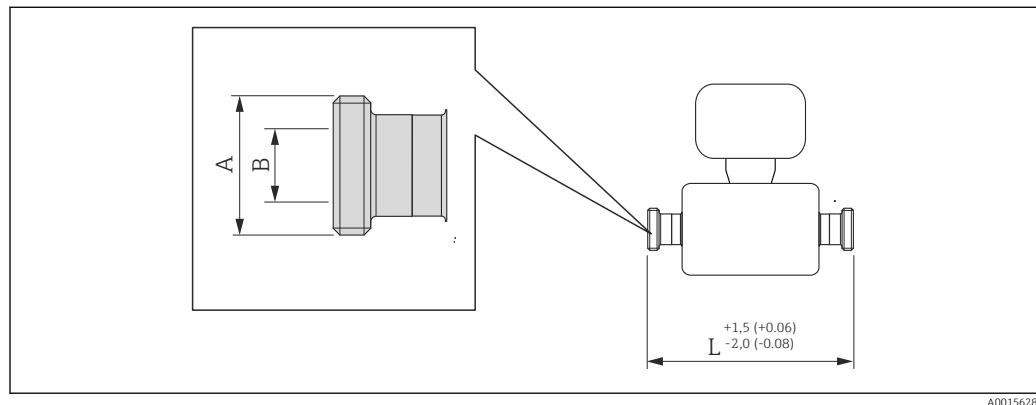

35 Engineering unit mm (in)

Threaded hygienic connection (sanitary connection) DIN 11851: titanium (order code for "Process connection", option KCW)			
DN [mm]	A [in]	B [mm]	L [mm]
8	Rd 34 × 1/8	16	427
15	Rd 34 × 1/8	16	463
15 FB	Rd 34 × 1/8	16	602
25	Rd 52 × 1/6	26	603
25 FB	Rd 52 × 1/6	26	736
40	Rd 65 × 1/6	38	731
40 FB	Rd 65 × 1/6	38	855
50	Rd 78 × 1/6	50	856
50 FB	Rd 78 × 1/6	50	1268


Threaded hygienic connection (sanitary connection) DIN 11851: titanium (order code for "Process connection", option KCW)			
DN [mm]	A [in]	B [mm]	L [mm]
80	Rd 110 × 1/4	81	1268

3A version available (order code for "Additional approval", option LP) in combination with Ra ≤ 0.8 µm (order code for "Measuring tube material", option CB)  
 FB = Full bore

Threaded hygienic connection (sanitary connection) DIN 11851 Rd 28 × 1/8": titanium (order code for "Process connection", option KAW)			
DN [mm]	A [in]	B [mm]	L [mm]
8	Rd 28 × 1/8	10	426
15	Rd 28 × 1/8	10	462

3A version available (order code for "Additional approval", option LP) in combination with Ra ≤ 0.8 µm (order code for "Measuring tube material", option CB)

DIN 11864-1 Form A (threaded hygienic connection)

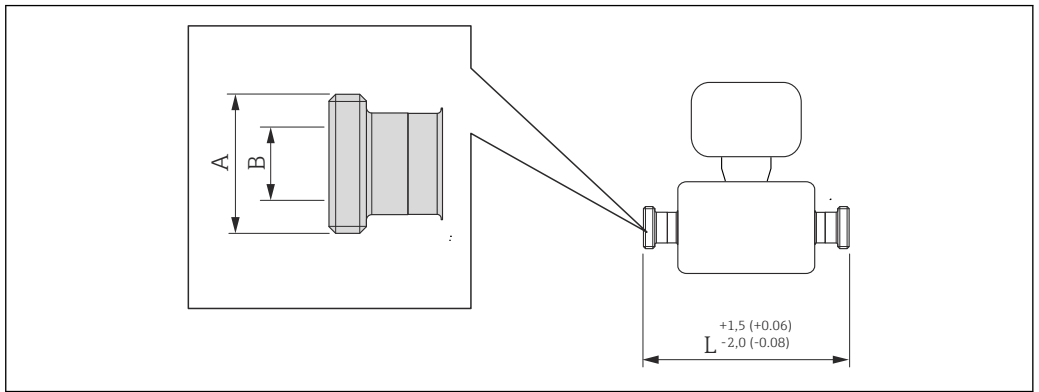

36 Engineering unit mm (in)


Threaded hygienic connection DIN 11864-1 Form A: titanium (order code for "Process connection", option KEW)			
DN [mm]	A [in]	B [mm]	L [mm]
8 <sup>1)</sup>	Rd 28 × 1/8	10	428
15	Rd 34 × 1/8	16	463
15 FB	Rd 34 × 1/8	16	602
25	Rd 52 × 1/6	26	603
25 FB	Rd 52 × 1/6	26	734
40	Rd 65 × 1/6	38	731
40 FB	Rd 65 × 1/6	38	855
50	Rd 78 × 1/6	50	856
50 FB	Rd 78 × 1/6	50	1268

Threaded hygienic connection DIN 11864-1 Form A: titanium (order code for "Process connection", option KEW)			
DN [mm]	A [in]	B [mm]	L [mm]
80	Rd 110 × 1/4	81	1268

3A version available (order code for "Additional approval", option LP) in combination with  $Ra \leq 0.8 \mu\text{m}$ ,  $Ra \leq 0.4 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)  
 FB = Full bore

1) DN 8 with DN 10 threaded hygienic connection as standard

DIN 11864-2 Form A (flange with groove)

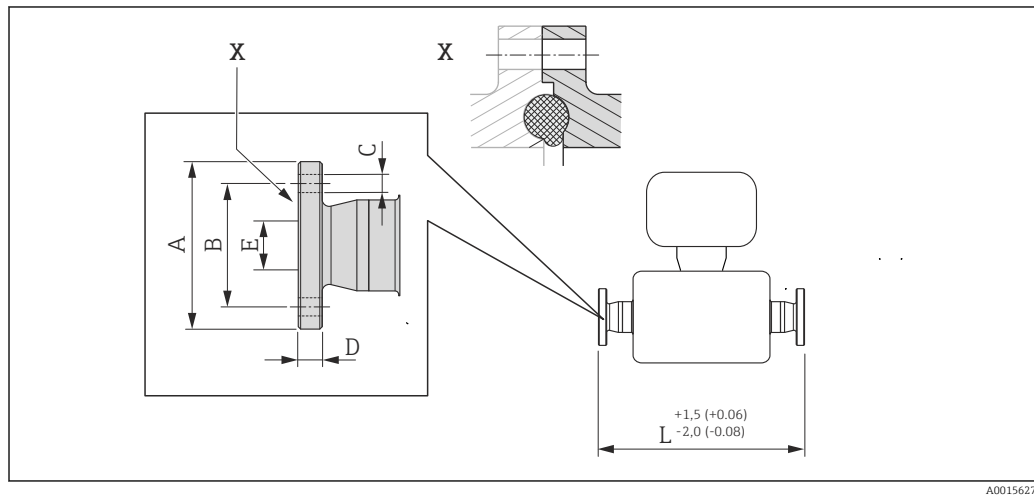

37 Detail X: Asymmetrical process connection; the part shown in gray is provided by the supplier. Engineering unit mm (in).


DIN 11864-2 Form A (flange with groove): titanium (order code for "Process connection", option KFW)						
DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
8 <sup>1)</sup>	54	37	4 × Ø9	10	10	449
15	59	42	4 × Ø9	10	16	485
25	70	53	4 × Ø9	10	26	625
40	82	65	4 × Ø9	10	38	753
50	94	77	4 × Ø9	10	50	874
80	133	112	8 × Ø11	12	81	1268

3A version available (order code for "Additional approval", option LP) in combination with  $Ra \leq 0.8 \mu\text{m}$ ,  $Ra \leq 0.4 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)  
 FB = Full bore

1) DN 8 with DN 15 flanges as standard



ISO 2853 (threaded hygienic connection)

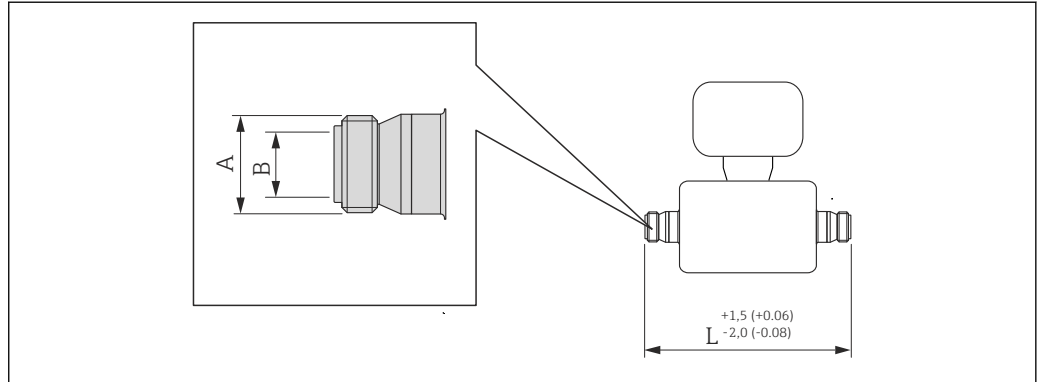

A0015623


38 Engineering unit mm (in)

Threaded hygienic connection ISO 2853: titanium (order code for "Process connection", option JSE)			
DN [mm]	A [mm]	B [mm]	L [mm]
8 <sup>1)</sup>	37.13	22.6	435
15	37.13	22.6	471
15 FB	37.13	22.6	610
25 FB	37.13	22.6	744
40	50.65	35.6	737
40 FB	50.65	35.6	859
50	64.16	48.6	856
50 FB	64.1	48.6	1268
80	91.19	72.9	1268

3A version available (order code for "Additional approval", option LP) in combination with Ra ≤ 0.8 µm, Ra ≤ 0.4 µm (order code for "Measuring tube material", option CB, CD)  
 FB = Full bore

1) DN 8 with DN 15 threaded hygienic connection as standard

SMS 1145 (threaded hygienic connection)

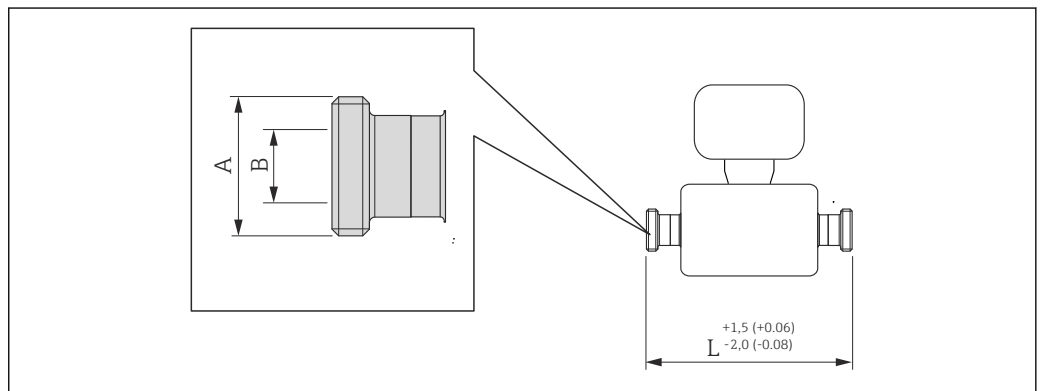

A0015628


39 Engineering unit mm (in)

Threaded hygienic connection SMS 1145: titanium (order code for "Process connection", option SCS)			
DN [mm]	A [in]	B [mm]	L [mm]
8	Rd 40 × 1/6	22.5	427
15	Rd 40 × 1/6	22.5	463
25	Rd 40 × 1/6	22.5	603
25 FB	Rd 40 × 1/6	22.5	736
40	Rd 60 × 1/6	35.5	738
40 FB	Rd 60 × 1/6	35.5	857
50	Rd 70 × 1/6	48.5	858
50 FB	Rd 70 × 1/6	48.5	1258
80	Rd 98 × 1/6	72	1268

3A version available ( $Ra \leq 0.8 \mu\text{m}$ ) (order code for "Additional approval", option LP)  
FB = Full bore

### Process connections in US units

Flange connections ASME B16.5

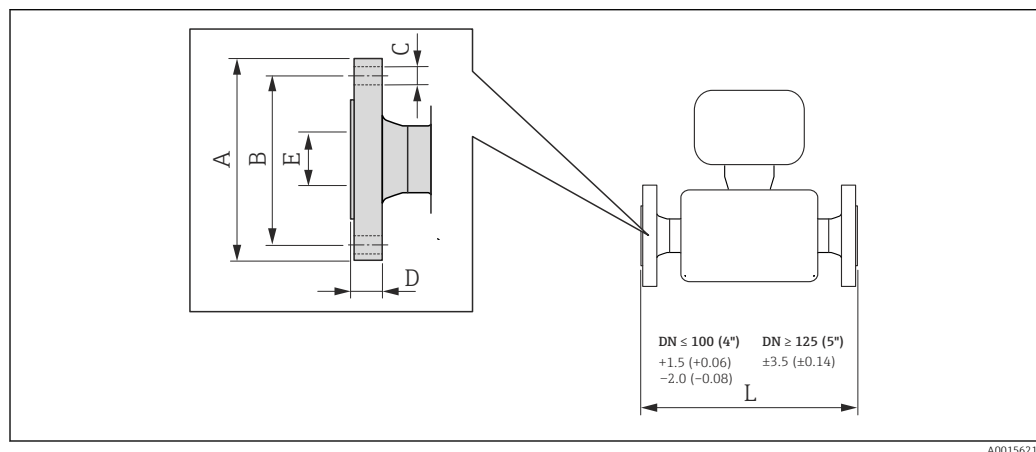

40 Engineering unit mm (in)

Flange according to ASME B16.5, Cl 150: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option AAW)						
Surface roughness (flange): $Ra$ 3.2 to 6.3 $\mu\text{m}$						
DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
$\frac{3}{8}$ <sup>1)</sup>	3.54	2.37	4 × Ø0.62	0.79	0.62	15.83
$\frac{1}{2}$	3.54	2.37	4 × Ø0.62	0.79	0.62	17.24
$\frac{1}{2}$ FB	3.54	2.37	4 × Ø0.62	0.75	0.67	22.52
1	4.33	3.13	4 × Ø0.62	0.91	1.05	22.76
1FB	4.33	3.13	4 × Ø0.62	0.87	1.01	27.56
1½	4.92	3.87	4 × Ø0.62	1.02	1.61	27.87
1½ FB	4.92	3.87	4 × Ø0.62	0.94	1.4	32.24
2	5.91	4.75	4 × Ø0.75	1.1	2.07	32.56
2FB	5.91	4.75	4 × Ø0.75	1.57	2.16	47.64

**Flange according to ASME B16.5, Cl 150: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option AAW)**

**Surface roughness (flange): Ra 3.2 to 6.3 µm**

DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
3	7.48	6.00	4 × Ø0.75	1.46	3.07	47.64

FB = Full bore

1) DN 3/8" with DN 1/2" flanges as standard;

**Flange according to ASME B16.5, Cl 300: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option ABW)**

**Surface roughness (flange): Ra 3.2 to 6.3 µm**

DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
3/8 <sup>1)</sup>	3.74	2.63	4 × Ø0.62	0.79	0.62	15.83
1/2	3.74	2.63	4 × Ø0.62	0.79	0.62	17.24
1/2FB	3.74	2.63	4 × Ø0.62	0.75	0.67	22.52
1	4.92	3.50	4 × Ø0.75	0.91	1.05	22.76
1FB	4.92	3.50	4 × Ø0.75	0.87	1.01	27.56
1 1/2	6.10	4.50	4 × Ø0.88	1.02	1.61	27.87
1 1/2 FB	6.10	4.50	4 × Ø0.88	0.94	1.4	32.24
2	6.50	5.00	8 × Ø0.75	1.1	2.07	32.56
2FB	6.50	5.00	8 × Ø0.75	1.69	2.16	47.64
3	8.27	6.63	8 × Ø0.88	1.65	3.07	47.64

FB = Full bore

1) DN 3/8" with DN 1/2" flanges as standard;

**Flange according to ASME B16.5, Cl 600: 1.4301 (304), wetted parts: titanium (order code for "Process connection", option ACW)**


**Surface roughness (flange): Ra 3.2 to 6.3 µm**

DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
3/8 <sup>1)</sup>	3.74	2.63	4 × Ø0.62	0.79	0.54	15.83
1/2	3.74	2.63	4 × Ø0.62	0.79	0.54	17.24
1/2FB	3.74	2.63	4 × Ø0.62	0.87	0.67	22.76
1	4.92	3.50	4 × Ø0.75	0.91	0.96	22.76
1FB	4.92	3.50	4 × Ø0.75	0.98	1.01	27.8
1 1/2	6.10	4.50	4 × Ø0.88	1.1	1.5	27.87
1 1/2 FB	6.10	4.50	4 × Ø0.88	1.14	1.4	32.48
2	6.50	5.00	8 × Ø0.75	1.3	1.94	32.76
2FB	6.50	5.00	8 × Ø0.75	1.81	2.16	47.64
3	8.27	6.63	8 × Ø0.88	2.09	2.9	48.11

FB = Full bore

1) DN 3/8" with DN 1/2" flanges as standard;

## Tri-Clamp

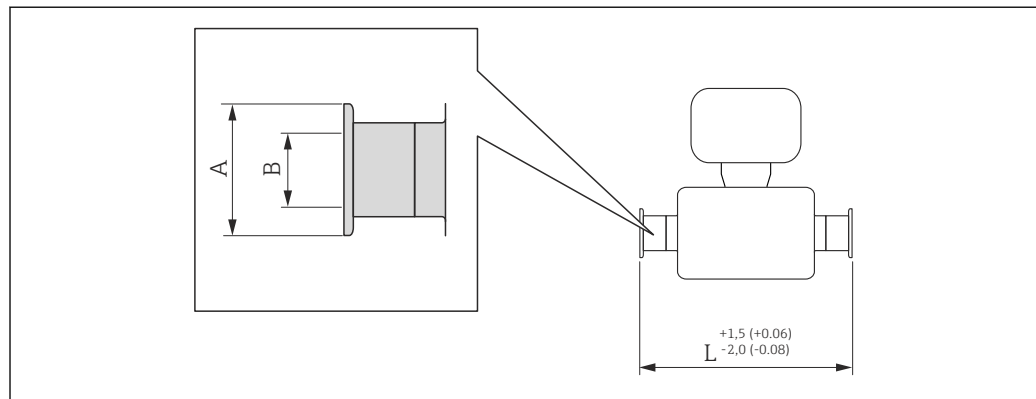

A0015625

41 Engineering unit mm (in)

1", 1½", 2" -Tri-Clamp for pipe size: titanium (order code for "Process connection", option FTW)				
DN [in]	Clamp [in]	A [in]	B [in]	L [in]
¾	1	1.98	0.87	16.81
½	1	1.98	0.87	18.23
½FB	see ¾" Tri-Clamp connection			
1	1	1.98	0.87	23.74
1FB	1	1.98	0.87	28.74
1½	1 ½	1.98	1.37	28.78
1½ FB	1 ½	1.98	1.37	33.43
2	2	2.52	1.87	33.46
2 FB <sup>1)</sup>	2 ½	3.05	2.37	49.92
3	3	3.58	2.87	49.92

3A version available (order code for "Additional approval", option LP) in combination with  $R_a \leq 32 \mu\text{m}$   $R_a \leq 16 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)  
FB = Full bore

1) Order code for "Process connection", option FRW


¾" Tri-Clamp: titanium (order code for "Process connection", option FEW)				
DN [in]	Clamp [in]	A [in]	B [in]	L [in]
¾	¾	0.98	0.63	16.77
½	¾	0.98	0.63	18.19
½FB	¾	0.98	0.63	23.7

3A version available (order code for "Additional approval", option LP) in combination with  $R_a \leq 32 \mu\text{m}$   $R_a \leq 16 \mu\text{m}$  (order code for "Measuring tube material", option CB, CD)  
FB = Full bore

<b>½" Tri-Clamp: titanium (order code for "Process connection", option FBW)</b>				
DN [in]	Clamp [in]	A [in]	B [in]	L [in]
¾	½	0.98	0.37	16.77
½	½	0.98	0.37	18.19

3A version available (order code for "Additional approval", option LP) in combination with Ra ≤ 32 µm Ra ≤ 16 µm (order code for "Measuring tube material", option CB, CD)

*Eccentric Tri-Clamp*

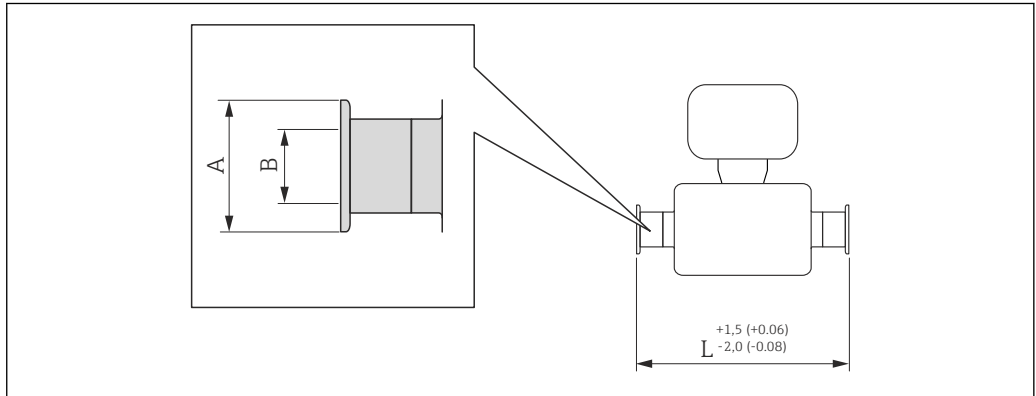


A0015625

42 Engineering unit mm (in)

<b>Eccentric Tri-Clamp: Titanium</b>					
DN [in]	Order code for "Process connection", option	Clamp [in]	A [in]	B [in]	L [in]
¾	FEA	½	0.98	0.37	16.81
½	FEC	¾	0.98	0.62	18.23
½FB	FEE	1	1.99	0.87	23.74
1	FEE	1	1.99	0.87	23.74
1FB	FEG	1½	1.99	1.37	28.74
1½	FEG	1½	1.99	1.37	28.74
1½ FB	FEJ	2	2.52	1.87	33.43
2	FEJ	2	2.52	1.87	33.43
2FB	FEL	2 ½	3.05	2.37	49.92
2FB	FEM	3	3.58	2.87	49.92
3	FEL	2 ½	3.05	2.37	49.92
3	FEM	3	3.58	2.87	49.92

3A version available (order code for "Additional approval", option LP) in combination with Ra ≤ 32 µm Ra ≤ 16 µm (order code for "Measuring tube material", option CB, CD)  
 FB = Full bore  
 Additional information on "Eccentric clamps" (→ 40)

SMS 1145 (threaded hygienic connection)

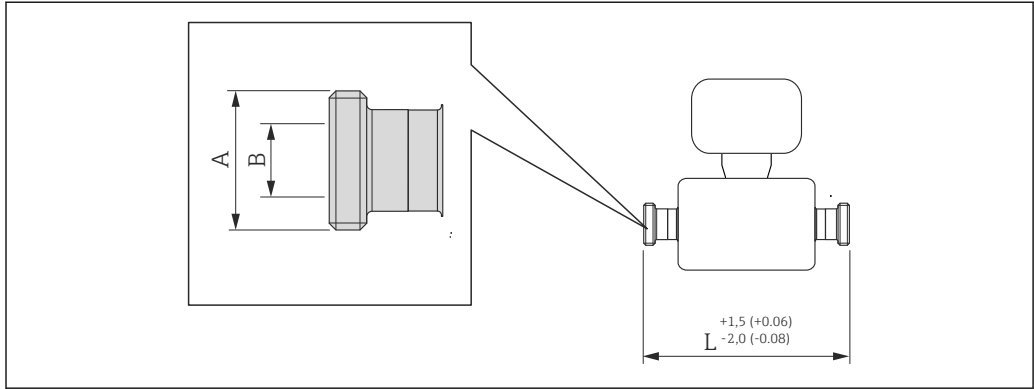

A0015628

43 Engineering unit mm (in)


Threaded hygienic connection SMS 1145: titanium (order code for "Process connection", option SCS)			
DN [in]	A [in]	B [in]	L [in]
3/8	Rd 40 × 1/6	0.89	16.81
1/2	Rd 40 × 1/6	0.89	18.23
1	Rd 40 × 1/6	0.89	23.74
1FB	Rd 40 × 1/6	0.89	28.98
1 1/2	Rd 60 × 1/6	1.4	29.06
1 1/2 FB	Rd 60 × 1/6	1.4	33.74
2	Rd 70 × 1/6	1.91	33.78
2FB	Rd 70 × 1/6	1.91	49.53
3	Rd 98 × 1/6	2.83	49.92

3A version available (order code for "Additional approval", option LP) in combination with Ra ≤ 32 µin (order code for "Measuring tube material", option CB)  
 FB = Full bore

Safety Barrier Promass 100

Top-hat rail EN 60715:

- TH 35 x 7.5
- TH 35 x 15

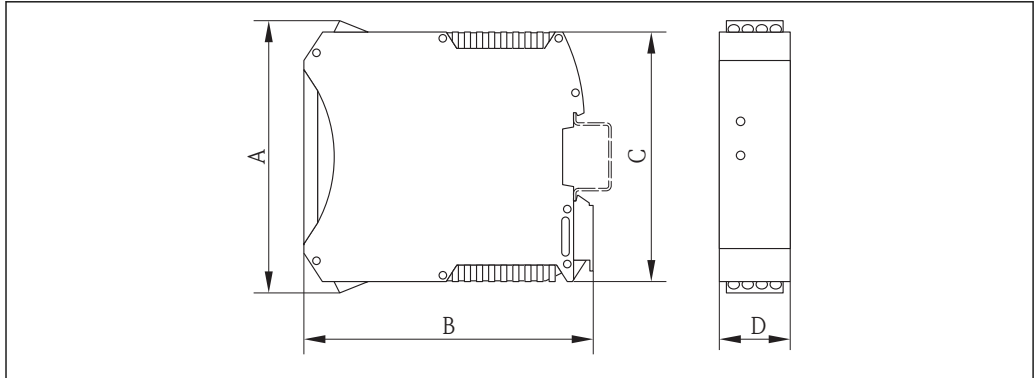


A0016777

A		B		C		D	
[mm]	[in]	[mm]	[in]	[mm]	[in]	[mm]	[in]
108	4.25	114.5	4.51	99	3.9	22.5	0.89

**Accessories**

*Purge connections / secondary containment monitoring*

Order code for "Sensor options", option CH

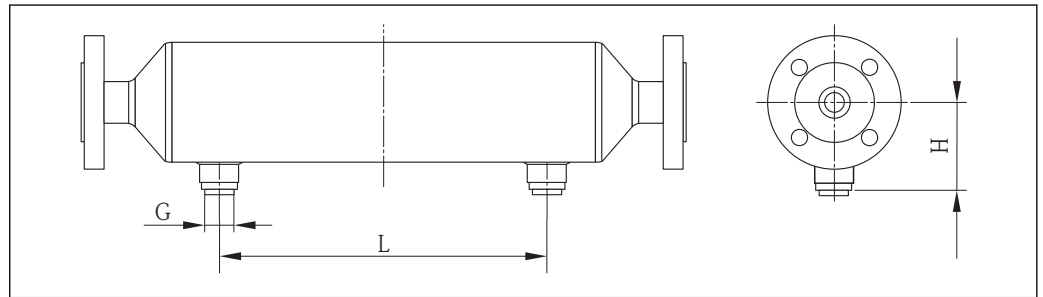

A0003321

DN		G	H		L	
[mm]	[in]	[in]	[mm]	[in]	[mm]	[in]
8	3/8	1/2-NPT	90.65	3.57	122	4.80
15	1/2	1/2-NPT	90.65	3.57	158	6.22
15FB	1/2FB	1/2-NPT	90.65	3.57	158	6.22
25	1	1/2-NPT	90.65	3.57	296	11.66
25FB	1FB	1/2-NPT	90.65	3.57	296	11.66
40	1 1/2	1/2-NPT	103.35	4.07	392	15.44
40FB	1 1/2 FB	1/2-NPT	103.35	4.07	392	15.44
50	2	1/2-NPT	117.75	4.64	488	19.22
50FB	2FB	1/2-NPT	145.5	5.73	814	32.40
80	3	1/2-NPT	145.5	5.73	814	32.40

**Weight**

**Compact version**

*Weight in SI units*

All values (weight) refer to devices with EN/DIN PN 40 flanges. Weight information in [kg].

DN [mm]	Weight [kg]
8	11
15	13
15 FB	19
25	20
25 FB	39
40	40
40 FB	65
50	67
50 FB	118

DN [mm]	Weight [kg]
80	122
FB = Full bore	

#### Weight in US units

All values (weight) refer to devices with EN/DIN PN 40 flanges. Weight information in [lbs].

DN [in]	Weight [lbs]
3/8	24
½	29
½ FB	42
1	44
1 FB	86
1½	88
1½ FB	143
2	148
2 FB	260
3	269
FB = Full bore	

#### Safety Barrier Promass 100


49 g (1.73 ounce)

#### Materials

##### Transmitter housing

- Order code for "Housing", option **A** "Compact, aluminum coated":  
Aluminum, AlSi10Mg, coated
- Order code for "Housing", option **B** "Compact, hygienic, stainless":  
Hygienic version, stainless steel 1.4301 (304)
- Order code for "Housing", option **C** "Ultra compact, hygienic, stainless":  
Hygienic version, stainless steel 1.4301 (304)

##### Cable entries/cable glands

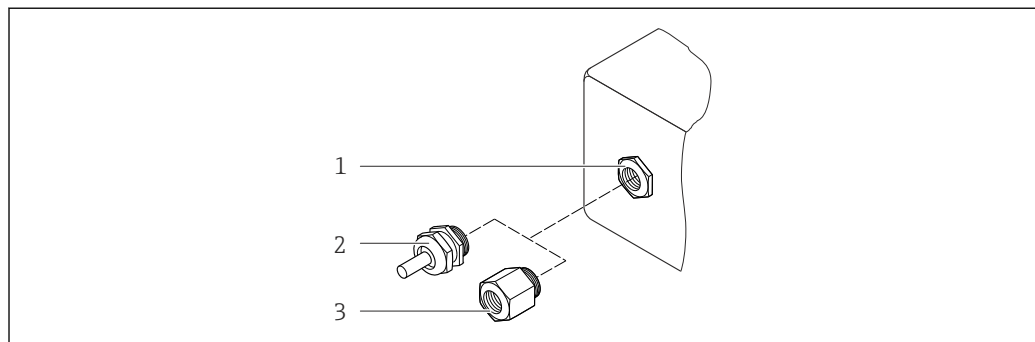

A0020640

#### 44 Possible cable entries/cable glands

- 1 Cable entry in transmitter housing, wall-mount housing or connection housing with internal thread M20 x 1.5
- 2 Cable gland M20 x 1.5
- 3 Adapter for cable entry with internal thread G ½" or NPT ½"



Order code for "Housing", option A "Compact, coated aluminum"

The various cable entries are suitable for hazardous and non-hazardous areas.

Cable entry/cable gland	Material
Cable gland M20 × 1.5	Nickel-plated brass
Adapter for cable entry with internal thread G ½"	
Adapter for cable entry with internal thread NPT ½"	

Order code for "Housing", option B "Compact, hygienic, stainless"

The various cable entries are suitable for hazardous and non-hazardous areas.

Cable entry/cable gland	Material
Cable gland M20 × 1.5	Stainless steel, 1.4404 (316L)
Adapter for cable entry with internal thread G ½"	
Adapter for cable entry with internal thread NPT ½"	

**Device plug**

Electrical connection	Material
Plug M12x1	<ul style="list-style-type: none"> <li>▪ Socket: Stainless steel, 1.4404 (316L)</li> <li>▪ Contact housing: Polyamide</li> <li>▪ Contacts: Gold-plated brass</li> </ul>

**Sensor housing**

- Acid and alkali-resistant outer surface
- Stainless steel 1.4301 (304)

**Measuring tubes**



Grade 9 titanium

**Surface quality:**

- Not polished
- Ra<sub>max</sub> = 0.8 µm (32 µin)
- Ra<sub>max</sub> = 0.4 µm (16 µin)

**Process connections**

- Flanges according to EN 1092-1 (DIN 2501) / according to ASME B16.5/ according to JIS:
  - Stainless steel 1.4301 (304)
  - Wetted parts: Grade 2 titanium
- All other process connections: Grade 2 titanium

 List of all available process connections (→  74)

**Seals**

Welded process connections without internal seals

**Safety Barrier Promass 100**

Housing: Polyamide

**Process connections**

- Flanges:
  - EN 1092-1 (DIN 2501)
  - EN 1092-1 (DIN 2512N)
  - ASME B16.5
  - JIS B2220
- Tri-Clamp (OD tubes)
- Clamp (eccentric) :
  - Tri-Clamp
- Threaded hygienic connection:
  - DIN 11851
  - SMS 1145
  - ISO 2853
  - DIN 11864-1 Form A
- Flange:
  - DIN 11864-2 Form A



For information on the materials of the process connections (→ 72)

## Operability

**Operating concept****Operator-oriented menu structure for user-specific tasks**

- Commissioning
- Operation
- Diagnostics
- Expert level

**Quick and safe commissioning**

- Individual menus for applications
- Menu guidance with brief explanations of the individual parameter functions

**Reliable operation**

- Operation in the following languages:
  - Via "FieldCare" operating tool:
    - English, German, French, Spanish, Italian, Chinese, Japanese
  - Via Web browser:
    - English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Bahasa (Indonesian), Vietnamese, Czech
- Uniform operating philosophy applied to operating tools and Web browser
- If replacing the electronic module, transfer the device configuration via the plug-in memory (HistoROM DAT) which contains the process and measuring device data and the event logbook. No need to reconfigure.
  - For devices with Modbus RS485, the data recovery function is implemented without the plug-in memory (HistoROM DAT).

**Efficient diagnostics increase measurement availability**

- Troubleshooting measures can be called up via the operating tools and Web browser
- Diverse simulation options
- Status indicated by several light emitting diodes (LEDs) on the electronic module in the housing compartment

**Local display**


The local display is only available with the following device version:  
Order code for "Display; Operation", option **B**: 4-line; via communication

**Display element**

- 4-line liquid crystal display with 16 characters per line.
- White background lighting; switches to red in event of device errors.
- Format for displaying measured variables and status variables can be individually configured.
- Permitted ambient temperature for the display: –20 to +60 °C (–4 to +140 °F). The readability of the display may be impaired at temperatures outside the temperature range.

**Remote operation****Via HART protocol**

This communication interface is present in the following device version:  
Order code for "Output", option **B**: 4-20 mA HART, pulse/frequency/switch output

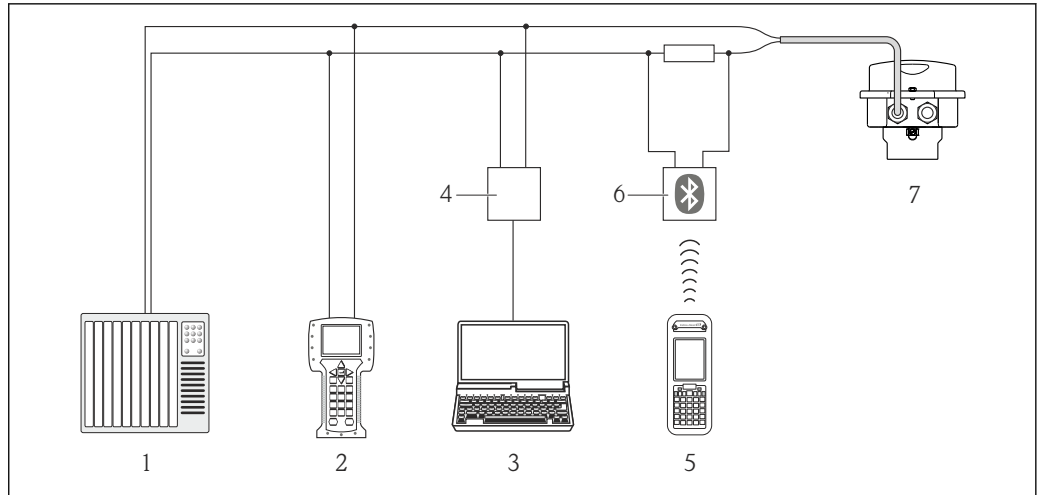


A0016948

45 Options for remote operation via HART protocol

- 1 Control system (e.g. PLC)
- 2 Field Communicator 475
- 3 Computer with operating tool (e.g. FieldCare, AMS Device Manager, SIMATIC PDM)
- 4 Commubox FXA195 (USB)
- 5 Field Xpert SFX350 or SFX370
- 6 VIATOR Bluetooth modem with connecting cable
- 7 Transmitter

**Via Ethernet-based fieldbus**

This communication interface is present in the following device version:  
 Order code for "Output", option **N**: EtherNet/IP

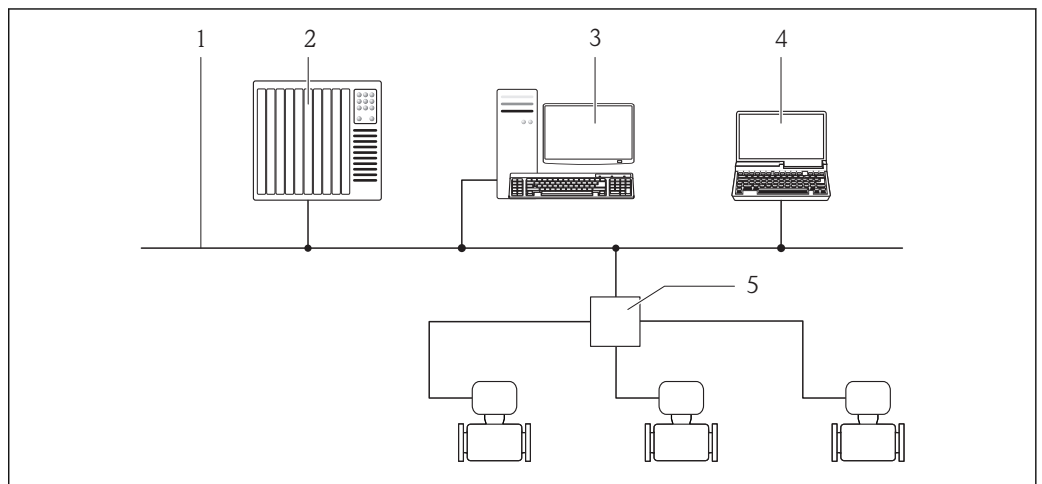


A0016961

- 1 Ethernet network
- 2 Automation system, e.g. "RSLogix" (Rockwell Automation)
- 3 Workstation for measuring device operation: with Add-on Profile Level 3 for "RSLogix 5000" (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 4 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or with "FieldCare" operating tool with COM DTM "CDI Communication TCP/IP"
- 5 Ethernet switch

**Via PROFIBUS DP network**

This communication interface is present in the following device version:  
 Order code for "Output", option **L**: PROFIBUS DP

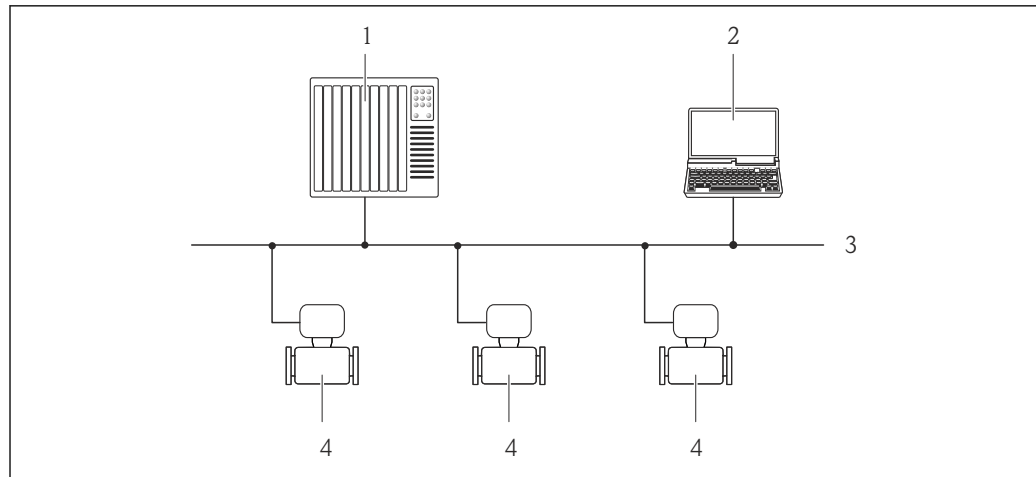

A0020903

- 1 Automation system
- 2 Computer with PROFIBUS network card
- 3 PROFIBUS DP network
- 4 Measuring device


## Service interface

### Service interface (CDI-RJ45)

This communication interface is present in the following device version:

- Order code for "Output", option B: 4-20 mA HART, pulse/frequency/switch output
- Order code for "Output", option L: PROFIBUS DP
- Order code for "Output", option N: EtherNet/IP

### HART

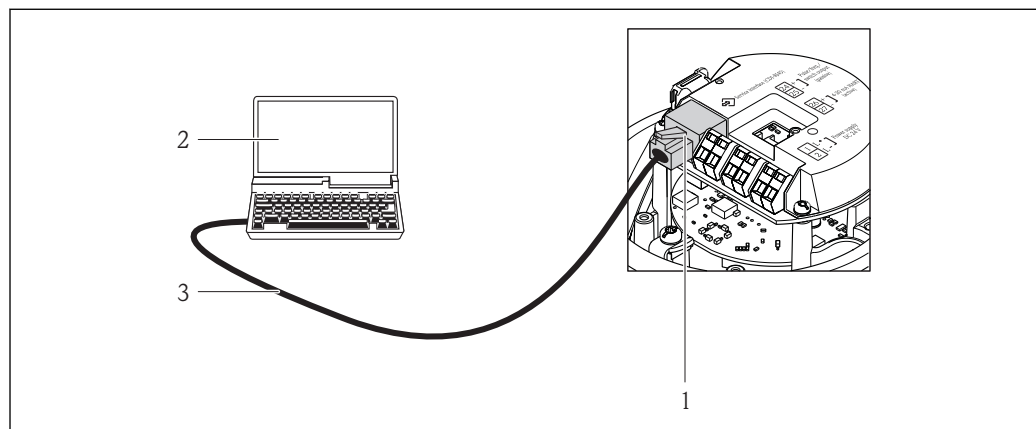


A0016926

46 Connection for the order code for "Output", option B: 4-20 mA HART, pulse/frequency/switch output

- 1 Service interface (CDI -RJ45) of the measuring device with access to the integrated Web server
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or with "FieldCare" operating tool with COM DTM "CDI Communication TCP/IP"
- 3 Standard Ethernet connecting cable with RJ45 plug

PROFIBUS DP

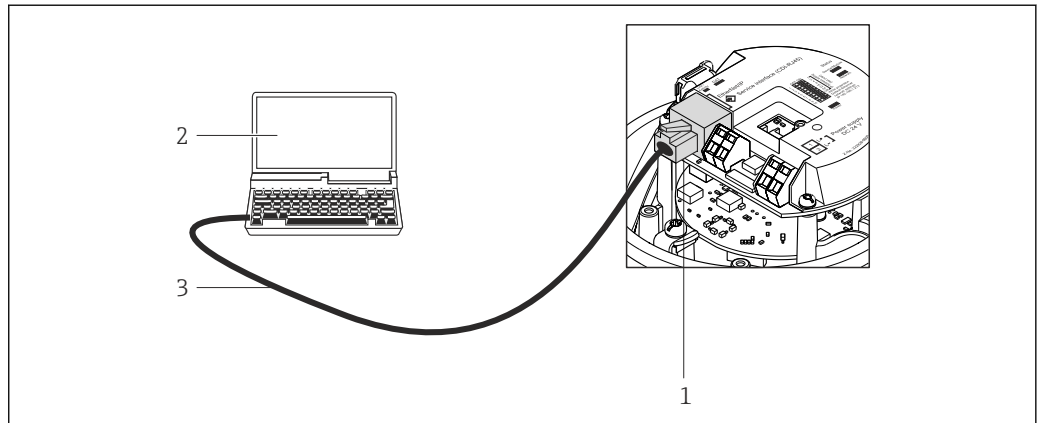


A0021270

47 Connection for order code for "Output", option L: PROFIBUS DP

- 1 Service interface (CDI -RJ45) of the measuring device with access to the integrated Web server
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or with "FieldCare" operating tool with COM DTM "CDI Communication TCP/IP"
- 3 Standard Ethernet connecting cable with RJ45 plug

EtherNet/IP

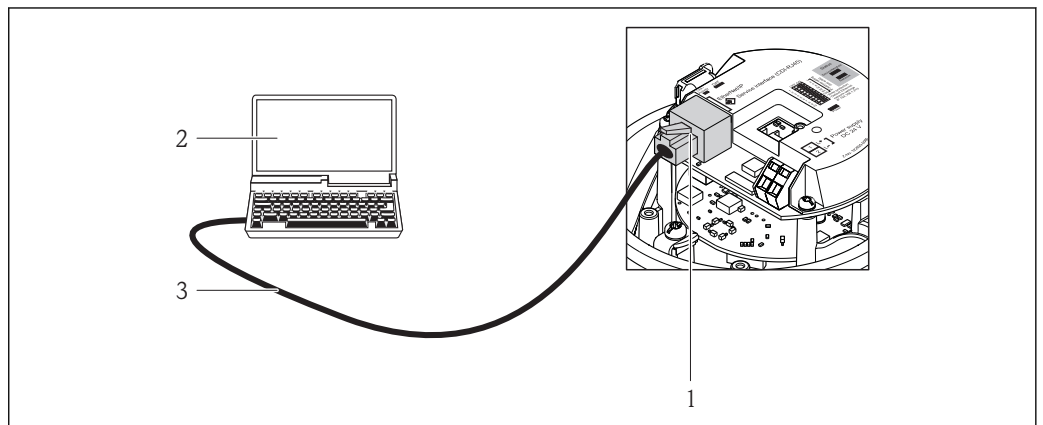


A0016940

48 Connection for order code for "Output", option N: EtherNet/IP

- 1 Service interface (CDI -RJ45) and EtherNet/IP interface of the measuring device with access to the integrated Web server
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or with "FieldCare" operating tool with COM DTM "CDI Communication TCP/IP"
- 3 Standard Ethernet connecting cable with RJ45 plug

**Service interface (CDI)**

This communication interface is present in the following device version:  
 Order code for "Output", option **M**: Modbus RS485

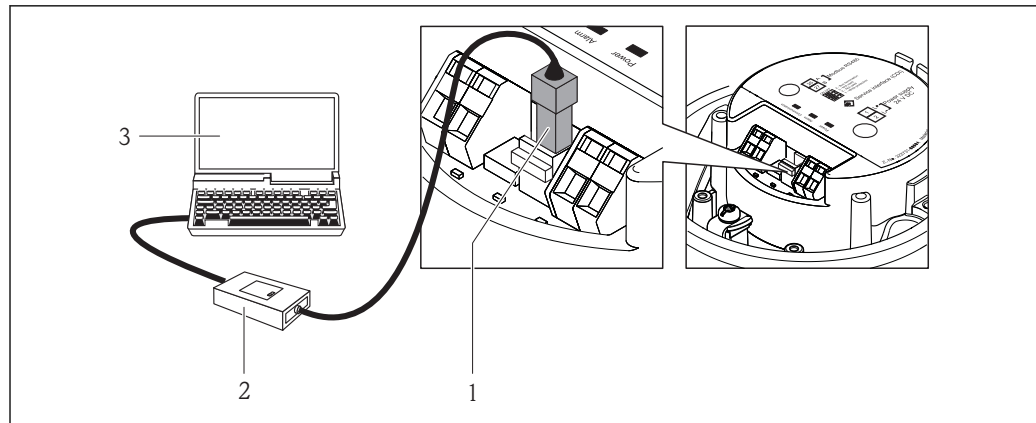

A0016925

- 1 Service interface (CDI) of the measuring device  
 2 Commubox FXA291  
 3 Computer with "FieldCare" operating tool with COM DTM "CDI Communication FXA291"

## Certificates and approvals

<b>CE mark</b>	<p>The measuring system is in conformity with the statutory requirements of the applicable EC Directives. These are listed in the corresponding EC Declaration of Conformity along with the standards applied.</p> <p>Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.</p>
<b>C-Tick symbol</b>	<p>The measuring system meets the EMC requirements of the "Australian Communications and Media Authority (ACMA)".</p>
<b>Ex approval</b>	<p>The measuring device is certified for use in hazardous areas and the relevant safety instructions are provided in the separate "Safety Instructions" (XA) document. Reference is made to this document on the nameplate.</p> <p><b>i</b> The separate Ex documentation (XA) containing all the relevant explosion protection data is available from your Endress+Hauser sales center.</p>

### ATEX/IECEX

Currently, the following versions for use in hazardous areas are available:

#### Ex ia

Category (ATEX)	Type of protection
II2G	Ex ia IIC T6...T1 Gb
II2G	Ex ia IIC T6...T1 Gb or Ex ia IIB T6...T1 Gb
II1/2G, II2D	Ex ia IIC T6...T1 Ga/Gb or Ex ia IIB T6...T1 Ga/Gb Ex tb IIIC Txxx Db
II2G, II2D	Ex ia IIC T6...T1 Gb or Ex ia IIB T6...T1 Gb Ex tb IIIC Txxx Db

#### Ex nA

Category (ATEX)	Type of protection
II3G	Ex nA IIC T6...T1 Gc or Ex nA IIC T5-T1 Gc

### cCSA<sub>US</sub>

Currently, the following versions for use in hazardous areas are available:

*IS (Ex i)*

- Class I Division 1 Groups ABCD
- Class II Division 1 Groups EFG and Class III

*NI (Ex nA)*

Class I Division 2 Groups ABCD

---

**Hygienic compatibility**

- 3A approval
  - EHEDG-tested
- 

**Certification PROFIBUS**

**PROFIBUS interface**

The measuring device is certified and registered by the PROFIBUS User Organization (PNO). The measuring system meets all the requirements of the following specifications:

- Certified in accordance with PROFIBUS PA Profile 3.02
  - The device can also be operated with certified devices of other manufacturers (interoperability)
- 

**Modbus RS485 certification**

The measuring device meets all the requirements of the MODBUS/TCP conformity test and has the "MODBUS/TCP Conformance Test Policy, Version 2.0". The measuring device has successfully passed all the test procedures carried out and is certified by the "MODBUS/TCP Conformance Test Laboratory" of the University of Michigan.

---

**EtherNet/IP certification**

The measuring device is certified and registered by the ODVA (Open Device Vendor Association). The measuring system meets all the requirements of the following specifications:

- Certified in accordance with the ODVA Conformance Test
  - EtherNet/IP Performance Test
  - EtherNet/IP PlugFest compliance
  - The device can also be operated with certified devices of other manufacturers (interoperability)
- 

**Pressure Equipment Directive**

The devices can be ordered with or without a PED approval. If a device with a PED approval is required, this must be explicitly stated in the order. For devices with nominal diameters less than or equal to DN 25 (1"), this is neither possible nor necessary.

- With the PED/G1/x (x = category) marking on the sensor nameplate, Endress+Hauser confirms compliance with the "Essential Safety Requirements" specified in Annex I of the Pressure Equipment Directive 97/23/EC.
  - Devices bearing this marking (PED) are suitable for the following types of medium:
    - Media in Group 1 and 2 with a vapor pressure greater than, or smaller and equal to 0.5 bar (7.3 psi)
    - Unstable gases
  - Devices not bearing this marking (PED) are designed and manufactured according to good engineering practice. They meet the requirements of Art.3 Section 3 of the Pressure Equipment Directive 97/23/EC. The range of application is indicated in tables 6 to 9 in Annex II of the Pressure Equipment Directive.
- 

**Other standards and guidelines**

- EN 60529  
Degrees of protection provided by enclosures (IP code)
  - IEC/EN 60068-2-6  
Environmental influences: Test procedure - Test Fc: vibrate (sinusoidal).
  - IEC/EN 60068-2-31  
Environmental influences: Test procedure - Test Ec: shocks due to rough handling, primarily for devices.
  - EN 61010-1  
Safety requirements for electrical equipment for measurement, control and laboratory use
  - IEC/EN 61326  
Emission in accordance with Class A requirements. Electromagnetic compatibility (EMC requirements).
  - NAMUR NE 21  
Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment
  - NAMUR NE 32  
Data retention in the event of a power failure in field and control instruments with microprocessors
  - NAMUR NE 43  
Standardization of the signal level for the breakdown information of digital transmitters with analog output signal.
-

- NAMUR NE 53  
Software of field devices and signal-processing devices with digital electronics
- NAMUR NE 80  
The application of the pressure equipment directive to process control devices
- NAMUR NE 105  
Specifications for integrating fieldbus devices in engineering tools for field devices
- NAMUR NE 107  
Self-monitoring and diagnosis of field devices
- NAMUR NE 131  
Requirements for field devices for standard applications
- NAMUR NE 132  
Coriolis mass meter

## Ordering information

Detailed ordering information is available from the following sources:

- In the Product Configurator on the Endress+Hauser website: [www.endress.com](http://www.endress.com) → Select country → Instruments → Select device → Product page function: Configure this product
- From your Endress+Hauser Sales Center: [www.endress.com/worldwide](http://www.endress.com/worldwide)

### Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
  - Depending on the device: Direct input of measuring point-specific information such as measuring range or operating language
  - Automatic verification of exclusion criteria
  - Automatic creation of the order code and its breakdown in PDF or Excel output format
  - Ability to order directly in the Endress+Hauser Online Shop

## Application packages

Many different application packages are available to enhance the functionality of the device. Such packages might be needed to address safety aspects or specific application requirements.

The application packages can be ordered from Endress+Hauser either directly with the device or subsequently. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: [www.endress.com](http://www.endress.com).

### Heartbeat Technology

Package	Description
Heartbeat Verification +Monitoring	<p><b>Heartbeat Monitoring:</b> Continuously supplies monitoring data, which are characteristic of the measuring principle, for an external condition monitoring system. This makes it possible to:</p> <ul style="list-style-type: none"> <li>■ Draw conclusions - using these data and other information - about the impact the measuring application has on the measuring performance over time.</li> <li>■ Schedule servicing in time.</li> <li>■ Monitor the product quality, e.g. gas pockets.</li> </ul> <p><b>Heartbeat Verification:</b> Makes it possible to check the device functionality on demand when the device is installed, without having to interrupt the process.</p> <ul style="list-style-type: none"> <li>■ Access via onsite operation or other operating interfaces, such as FieldCare for instance.</li> <li>■ Documentation of device functionality within the framework of manufacturer specifications, for proof testing for instance.</li> <li>■ End-to-end, traceable documentation of the verification results, including report.</li> <li>■ Makes it possible to extend calibration intervals in accordance with operator's risk assessment.</li> </ul>



**Concentration**

Package	Description
Concentration measurement and special density	<p><b>Calculation and outputting of fluid concentrations</b></p> <p>Many applications use density as a key measured value for monitoring quality or controlling processes. The device measures the density of the fluid as standard and makes this value available to the control system.</p> <p>The "Special Density" application package offers high-precision density measurement over a wide density and temperature range particularly for applications subject to varying process conditions.</p> <p>With the help of the "Concentration Measurement" application package, the measured density is used to calculate other process parameters:</p> <ul style="list-style-type: none"> <li>▪ Temperature-compensated density (reference density).</li> <li>▪ Percentage mass of the individual substances in a two-phase fluid. (Concentration in %).</li> <li>▪ Fluid concentration is output with special units (°Brix, °Baumé, °API, etc.) for standard applications.</li> </ul> <p>The measured values are output via the digital and analog outputs of the device.</p>

**Viscosity**


Package	Description
Viscosity measurement	<p><b>In-line and real-time viscosity measurement</b></p> <p>Promass I with the "Viscosity" application package also measures the real-time viscosity of the fluid directly in the process, in addition to measuring the mass flow/volume flow/ temperature and density.</p> <p>The following viscosity measurements are performed on liquids:</p> <ul style="list-style-type: none"> <li>▪ Dynamic viscosity</li> <li>▪ Kinematic viscosity</li> <li>▪ Temperature-compensated viscosity (kinematic and dynamic) in relation to the reference temperature</li> </ul> <p>Viscosity measurement can be used for Newtonian and non-Newtonian applications and supplies accurate measured data irrespective of the flow, even under difficult conditions.</p>

## Accessories



Various accessories, which can be ordered with the device or subsequently from Endress+Hauser, are available for the device. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: [www.endress.com](http://www.endress.com).






**Device-specific accessories**

**For the sensor**



Accessories	Description
Heating jacket	<p>Is used to stabilize the temperature of the fluids in the sensor. Water, water vapor and other non-corrosive liquids are permitted for use as fluids. If using oil as a heating medium, please consult with Endress+Hauser.</p> <p> For details, see Operating Instructions BA00099D</p>

**Communication-specific accessories**



Accessories	Description
Commubox FXA195 HART	<p>For intrinsically safe HART communication with FieldCare via the USB interface.</p> <p> For details, see "Technical Information" TI00404F</p>
HART Loop Converter HMX50	<p>Is used to evaluate and convert dynamic HART process variables to analog current signals or limit values.</p> <p> For details, see "Technical Information" TI00429F and Operating Instructions BA00371F</p>

Wireless HART adapter SWA70	<p>Is used for the wireless connection of field devices. The WirelessHART adapter can be easily integrated into field devices and existing infrastructures, offers data protection and transmission safety and can be operated in parallel with other wireless networks with minimum cabling complexity.</p> <p> For details, see Operating Instructions BA00061S</p>
Fieldgate FXA320	<p>Gateway for the remote monitoring of connected 4-20 mA measuring devices via a Web browser.</p> <p> For details, see "Technical Information" TI00025S and Operating Instructions BA00053S</p>
Fieldgate FXA520	<p>Gateway for the remote diagnostics and remote configuration of connected HART measuring devices via a Web browser.</p> <p> For details, see "Technical Information" TI00025S and Operating Instructions BA00051S</p>
Field Xpert SFX350	<p>Field Xpert SFX350 is a mobile computer for commissioning and maintenance. It enables efficient device configuration and diagnostics for HART and FOUNDATION Fieldbus devices in the <b>non-Ex area</b>.</p> <p> For details, see Operating Instructions BA01202S</p>
Field Xpert SFX370	<p>Field Xpert SFX370 is a mobile computer for commissioning and maintenance. It enables efficient device configuration and diagnostics for HART and FOUNDATION Fieldbus devices in the <b>non-Ex area</b> and the <b>Ex area</b>.</p> <p> For details, see Operating Instructions BA01202S</p>


## Service-specific accessories

Accessories	Description
Applicator	<p>Software for selecting and sizing Endress+Hauser measuring devices:</p> <ul style="list-style-type: none"> <li>■ Calculation of all the necessary data for identifying the optimum flowmeter: e.g. nominal diameter, pressure loss, accuracy or process connections.</li> <li>■ Graphic illustration of the calculation results</li> </ul> <p>Administration, documentation and access to all project-related data and parameters over the entire life cycle of a project.</p> <p>Applicator is available:</p> <ul style="list-style-type: none"> <li>■ Via the Internet: <a href="https://wapps.endress.com/applicator">https://wapps.endress.com/applicator</a></li> <li>■ On CD-ROM for local PC installation.</li> </ul>
W@M	<p>Life cycle management for your plant</p> <p>W@M supports you with a wide range of software applications over the entire process: from planning and procurement, to the installation, commissioning and operation of the measuring devices. All the relevant device information, such as the device status, spare parts and device-specific documentation, is available for every device over the entire life cycle.</p> <p>The application already contains the data of your Endress+Hauser device. Endress+Hauser also takes care of maintaining and updating the data records.</p> <p>W@M is available:</p> <ul style="list-style-type: none"> <li>■ Via the Internet: <a href="http://www.endress.com/lifecyclemanagement">www.endress.com/lifecyclemanagement</a></li> <li>■ On CD-ROM for local PC installation.</li> </ul>
FieldCare	<p>FDT-based plant asset management tool from Endress+Hauser. It can configure all smart field units in your system and helps you manage them. By using the status information, it is also a simple but effective way of checking their status and condition.</p> <p> For details, see Operating Instructions BA00027S and BA00059S</p>
Commubox FXA291	<p>Connects Endress+Hauser field devices with a CDI interface (= Endress+Hauser Common Data Interface) and the USB port of a computer or laptop.</p> <p> For details, see "Technical Information" TI00405C</p>

**System components**

Accessories	Description
Memograph M graphic display recorder	The Memograph M graphic display recorder provides information on all relevant measured variables. Measured values are recorded correctly, limit values are monitored and measuring points analyzed. The data are stored in the 256 MB internal memory and also on a SD card or USB stick.  For details, see "Technical Information" TI00133R and Operating Instructions BA00247R
iTEMP	The temperature transmitters can be used in all applications and are suitable for the measurement of gases, steam and liquids. They can be used to read in the fluid temperature.  For details, see "Fields of Activity", FA00006T

## Documentation

-  For an overview of the scope of the associated Technical Documentation, refer to the following:
- The CD-ROM provided for the device (depending on the device version, the CD-ROM might not be part of the delivery!)
  - The *W@M Device Viewer* : Enter the serial number from the nameplate ([www.endress.com/deviceviewer](http://www.endress.com/deviceviewer))
  - The *Endress+Hauser Operations App*: Enter the serial number from the nameplate or scan the 2-D matrix code (QR code) on the nameplate.

**Standard documentation**

**Brief Operating Instructions**

Measuring device	Documentation code
Promass I 100	KA01117D

**Operating Instructions**

Measuring device	Documentation code			
	HART	PROFIBUS DP	Modbus RS485	EtherNet/IP
Promass I 100	BA01190D	BA01251D	BA01058D	BA01066D

**Supplementary device-dependent documentation**

**Safety Instructions**


Contents	Documentation code
ATEX/IECEX Ex i	XA00159D
ATEX/IECEX Ex nA	XA01029D
cCSAus IS	XA00160D
INMETRO Ex i	XA01219D
INMETRO Ex nA	XA01220D
NEPSI Ex i	XA01249D
NEPSI Ex nA	XA01262D

**Special Documentation**

Contents	Documentation code
Information on the Pressure Equipment Directive	SD00142D
Modbus RS485 Register Information	SD00154D

Contents	Documentation code
Concentration Measurement	SD01152D
Viscosity Measurement	SD01151D
Heartbeat Technology	SD01153D

### Installation Instructions

Contents	Documentation code
Installation Instructions for spare part sets	Specified for each individual accessory (→  81)

## Registered trademarks

### HART®

Registered trademark of the HART Communication Foundation, Austin, USA

### PROFIBUS®

Registered trademark of the PROFIBUS User Organization, Karlsruhe, Germany

### Modbus®

Registered trademark of SCHNEIDER AUTOMATION, INC.

### EtherNet/IP™

Trademark of ODVA, Inc.

### Microsoft®

Registered trademark of the Microsoft Corporation, Redmond, Washington, USA

### TRI-CLAMP®

Registered trademark of Ladish & Co., Inc., Kenosha, USA

### Applicator®, FieldCare®, Field Xpert™, HistoROM®, TMB®, Heartbeat Technology™

Registered or registration-pending trademarks of the Endress+Hauser Group

[www.addresses.endress.com](http://www.addresses.endress.com)