Light section sensor for object measurement







200 ... 600 mm





- Light section sensor for object measurement (width, height and position measurement)
- Measurement time 10ms
- Measurement range: 200 ... 600mm
- Length of laser line: max. 140mm
- Integrated analog interface
- Configuration via Fast Ethernet
- OLED display with key pad for alignment aid and status display: "set inspection task"
- Measurement value display in mm on OLED display as an alignment aid
- Up to 4 measurement fields / 8 detection fields with logic operation option
- Up to 16 inspection tasks
- Activation input, trigger input, cascading output












Accessories:


(available separately)

- Mounting systems BT 56, BT 59
- Cable with M12 connector (K-D ...)
- Configuration memory K-DS M12A-8P-0,75m-LxS36-CP

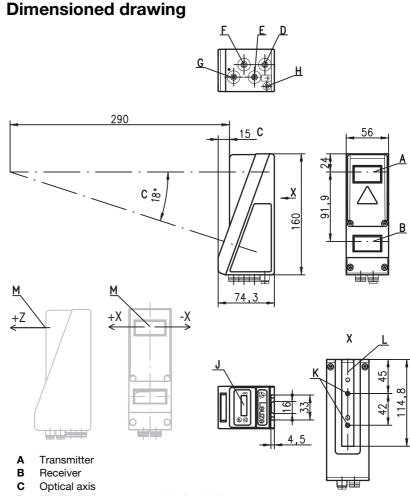

- D X1: M12x1 connector, 8-pin, A coded
- E X2: M12x1 socket, 4-pin, D coded
- F X3: M12x1 socket, 8-pin, A coded (LES 36 HI/VC6)
- G X4: M12x1 socket, 5-pin, A coded (LES 36 HI/VC6)
- **H** FE screw
- J OLED display and membrane keyboard
- K M4 thread, 4.5 deep
- L Holder for mounting system BT 56 / BT 59
- M Zero point and orientation of the coordinate system for measurement data

Measurement range, typical

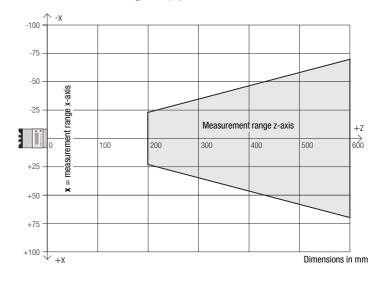

Specifications

Optical data

Measurement range 1) 200 ... 600mm (z direction) Light source laser Wavelength 658nm (visible red light)

Max. output power < 8mW

< 3ms (adjustable from 0.1 ms ... 1.31 ms) approx. 170x1.5mm at 600mm Pulse duration

Laser line

Error limits (relative to measurement distance)

Resolution in **x** direction ^{2) 3)}
Resolution in **z** ²⁾direction ³⁾ 0.2 ... 0.6mm 0.1 ... 09mm Linearity in **z** direction ³⁾
Repeatability in **z** direction ³⁾ ≤ ±0.5% ≤ 0.25 % B/W detection thresh. (6 ... 90% rem.) ≤ 0.5 %

Object detection

Minimum object size in x direction 4) 0.6 ... 2mm Minimum object size in **z** direction ²⁾ 0.4 ... 3mm

Timing

≥10ms (configurable) Measurement time

Delay before start-up approx. 1.5s

Electrical data

18 ... 30 VDC (incl. residual ripple) \leq 15% of U_B Operating voltage U_B 5)

Residual ripple ≤ 200 mA Open-circuit current Ethernet interface **UDP**

Switching outputs

4 / 100mA / push-pull ⁶⁾ on X3 (LES 36 HI/VC6 only) 1 (ready) / 100mA / push-pull ⁶⁾ on X1 1 (cascading) / 100mA / push-pull ⁶⁾ on X1

(selection of inspection task) on X3 (LES 36 HI/VC6 only) Inputs

(trigger) on X1 (activation) on X1

≥ (U_B-2V)/≤ 2V Signal voltage high/low

Analog output (only LES 36 HI/VC6)

voltage 1 ... 10V, $R_L \ge 2k\Omega$ current 4 ... 20mA, $R_L \le 500\Omega$ Analog output

Indicators

Green LED continuous light ready no voltage off

Yellow LED continuous light Ethernet connection available

flashing Ethernet data transmission active no Ethernet connection available

Mechanical data

aluminum frame with plastic cover Housing

glass 620g Optics cover Weight Connection type M12 connector

Environmental data

Ambient temp. (operation/storage) Protective circuit 7) -30°C ... +50°C/-30°C ... +70°C 1, 2, 3 VDE safety class III, protective extra-low voltage

Protection class

2M (according to EN 60825-1 and 21 CFR 1040.10 with Laser Laser class

Notice No. 50) IEC/EN 60947-5-2 Standards applied

Certifications UL 508, C22.2 No.14-13 5) 8)

Luminosity coefficient 6% ... 90%, entire detection range, at 20°C after 30minutes warmup time, medium range U_B

Minimum and maximum value depend on measurement distance

Reflectivity 90 %, identical object, identical environment conditions, measurement object ≥ 50x50mm²

Minimum value, depends on distance and object, requires testing under application conditions

For UL applications: for use in class 2 circuits according to NEC only

The push-pull switching outputs must not be connected in parallel

1=transient protection, 2=polarity reversal protection, 3=short circuit protection for all outputs, requires external protective circuit for inductive loads


These sensors shall be used with UL Listed Cable assemblies rated 30V, 0.5A min, in the field installation, or equivalent (categories: CYJV/CYJV7 or PVVA/PVVA7)

Tables

LED	State	Display during measurement operation
green	continu- ous light	Sensor ready
	off	Sensor not ready
yellow	continu-	Ethernet connec-
	ous light	tion established
	flashing	Ethernet data
		transmission
		active
	off	No Ethernet
		connection


Diagrams

Line length/measurement range (typical)



- A Measurement range
- B Line length

Resolution (typical)



Remarks

Operate in accordance with intended use!

- This product is not a safety sensor and is not intended as personnel
- operation by competent persons.
- Only use the product in accordance with the intended use.

Warmup time:

After a warmup time of 30 min., the light section sensor has reached the operating temperature required for an optimum object measurement

2014/06

LES 36 HI... - 02

Light section sensor for object measurement

Interface assignments

X1 - logic and power			
Pin No.	Signal	Color	
1	+24VDC	WH	
2	InAct (activation)	BN	
3	GND	GN	
4	OutReady (ready)	YE	
5	InTrig (trigger)	GY	
6	OutCas (cascading)	PK	
7	do not connect	BU	
8	do not connect	RD	
O C. MAO II - A - III			

M nia-8	12	nlua	Δ	coded

X2 - Ethernet			
Pin No.	Signal	Color	
1	Tx+	YE	
2	Rx+	WH	
3	Tx-	OR	
4	Rx-	BU	

4-pin M12 socket, D coded

X3 - logic (LES 36 HI/VC6 only)		
Pin No.	Signal	Color
1	Out4	WH
2	Out3	BN
3	GND	GN
4	Out2	YE
5	Out1	GY
6	InSel3 1)	PK
7	InSel2 1)	BU
8	InSel1 1)	RD

8-pin M12 socket, A coded

X4 - Analog Out			
Pin No. Signal Explanation Co			Color
1	n.c.	Not connected	BN
2	4-20 mA	Analog current output	WH
3	AGND	Reference potential	BU
4	1-10V	Analog voltage output	BK
5	FE	Functional earth	GY

⁵⁻pin M12 socket, A coded

1) The three InSel1-3 switching inputs are used to select inspection tasks 0-7. "000" means inspection task 0, "001" inspection task 1, etc. The changeover time between two inspection tasks is < 100ms

Order guide

Part no. Designation Line Range Sensor

50111329 LES 36HI/VC6 with analog voltage/current output and binary inputs/outputs

Laser safety notices



ATTENTION, LASER RADIATION - LASER CLASS 2M

Never look directly into the beam or point the beam in the direction of telescope users!

The device fulfills the EN 60825-1:2008-05 (IEC 60825-1:2007) safety regulations for a product in **laser class 2M** as well as the U.S. 21 CFR 1040.10 regulations with deviations corresponding to "Laser Notice No. 50" from June 24th, 2007.

- Never look directly into the laser beam or in the direction of reflecting laser beams!
 If you look into the beam path over a longer time period, there is a risk of injury to the retina.
- ♥ Do not point the laser beam of the device at persons!
- 🔖 Intercept the laser beam with an opaque, non-reflective object if the laser beam is accidentally directed towards a person.
- \$ When mounting and aligning the device, avoid reflections of the laser beam off reflective surfaces!
- CAUTION! Use of controls or adjustments or performance of procedures other than specified herein may result in hazardous light exposure.
 - The use of optical instruments or devices (e.g., magnifying glasses, binoculars) with the product will increase eye hazard.
- Adhere to the applicable legal and local regulations regarding protection from laser beams acc. to EN 60825 (IEC 60825) in its latest version.

There are no user-serviceable parts inside the device.

Repairs must only be performed by Leuze electronic GmbH + Co. KG.


NOTICE


Affix laser information and warning signs!

Laser information and warning signs are affixed to the device(see ①). In addition, self-adhesive laser information and warning signs (stick-on labels) are supplied in several languages (see ②).

- Affix the laser information sheet with the language appropriate for the place of use to the device. When using the device in the US, use the stick-on label with the "Complies with 21 CFR 1040.10" notice.
- Affix the laser information and warning signs near the device if no signs are attached to the device (e.g. because the device is too small) or if the attached laser information and warning signs are concealed due to the installation position.

Affix the laser information and warning signs so that they are legible without exposing the reader to the laser radiation of the device or other optical radiation.

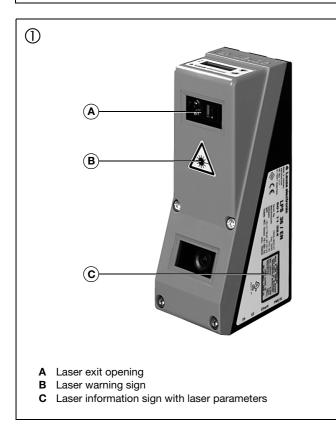

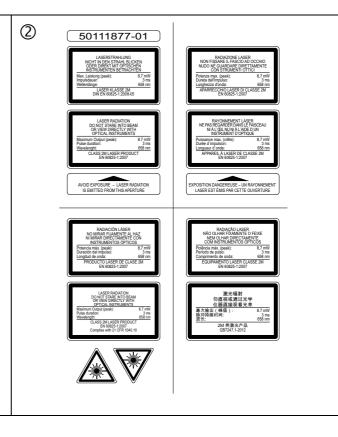

LES 36 Hl... - 02 2014/06

Light section sensor for object measurement

Configuration - Establish connection to PC

The LES is configured via a PC using the LESsoft program before it is integrated into the process control.

In order to be able to establish an UDP communication with the PC, the IP address of your PC and the IP address of the LES must lie in the same address range. The LES has no built-in DHCP client, so that you need to set the address manually. This is done the easiest way via the PC.

∧ Notice!

If you are using a desktop firewall, please ensure that the control can communicate with the LES via the Ethernet interface on ports 9008 and 5634 using UDP. Furthermore, the firewall must allow ICMP echo messages to pass through for the connection test (ping).

If the PC is usually connected to a network using DHCP address allocation, the easiest way to access the LES is by applying an alternative configuration in the TCP/IP settings of the PC and connecting the LES directly to the PC.

♦ Check the network address of the LES by pressing the → button during normal operation of the LES twice in succession, then by pressing ▼ twice and followed by pressing the → button again.

This will take you to the Ethernet submenu and enable you to read the current settings of the LES consecutively when pressing ▼ repeatedly.

Make a note of the values for IP-Address and Net Mask Addr..

The value in Net Mask Addr. specifies which digits of the IP address of the PC and LES must match so that they can communicate with each other.

Address of the LES	Net mask	Address of the PC
192.168.060.003	255.255.255.0	192.168.060.xxx
192.168.060.003	255.255.0.0	192.168.xxx.xxx


Instead of xxx you can now allocate any numbers between 000 and 255 to your PC, but NOT THE SAME numbers as contained in the address of the LES.

For example 192.168.060.110 (but not 192.168.060.003!). If LES and PC have the same IP address, they cannot communicate with each other.

Configuring the IP address for a PC

- ♦ Log in to your PC as an administrator.
- ♥ Using Start->System control go to the Network connections (Windows XP) menu or to the Network center and release center (Windows Vista) menu.
- There select the LAN connection and bring up the associated Features page by right clicking with the mouse.
- Select the Internet protocol (TCP/IP) (by scrolling down, if necessary) and click on Properties.
- ♦ In the Internet protocol (TCP/IP) Properties window select the Alternate configuration tab.
- Configure the IP address of the PC in the address range of the LES. Attention: do not use the same as for the LES!
- ♦ Set the Subnet mask of the PC to the same value as the one for the LES.
- ♦ Close the configuration dialog by confirming all windows using 0K.
- Connect the interface X2 of the LES directly to the LAN port of your PC. Use a KB ET-...-SA-RJ45 cable for the connection.

The PC will first try to establish a network connection via the automatic configuration. This will take a few seconds. Following that the alternative configuration, which you have just set up, is activated, and thus the PC can communicate with the LES. Information about configuring the LES using **LESsoft** software can be found in the Technical Description.

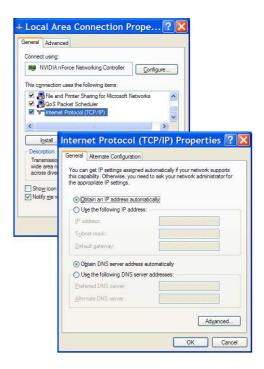


Commissioning

Notice!

П

The LES 36HI/VC6, like all other models, is configured via Ethernet with the LESsoft software.

- 1. Configuring the LES see chapter 8 of the Technical Description.
- Programming process control see chapter 9 of the Technical Description. or
- 3. Connecting the switching inputs and outputs accordingly see chapter 6 of the Technical Description.
- 4. Adapt the IP configuration of the LES via the display in such a way that it can communicate with LESsoft. Here you can change network address and associated net mask as well as the ports via which the LES communicates with process control. The values set via the display are not accepted immediately; they are not effective until the sensor is switched on again.
- 5. You can check the connection by entering the IP address data into **LESsoft** in the IP Configuration area and clicking on the Check Connectivity button.

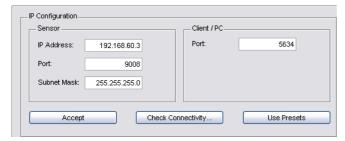

- 6. Configure LES with LESsoft.
- 7. Connect LES to the process control.
- 8. Establish connections for activation, triggering and cascading, if necessary.

LES 36 HI... - 02 2014/06

Light section sensor for object measurement

Installing the configuration software

System requirements

The PC used should meet the following requirements:

- Pentium® or faster Intel® processor > 1.5 GHz (Pentium 4, Celeron, Xeon) or compatible models by AMD® (Athlon 64, Opteron, Sempron). The processor must support the SSE2 instruction set.
- At least 512 MB free main memory (RAM), 1024 MB recommended
- CD-ROM drive
- Hard disk with at least 1 GB available memory.
- Ethernet port
- Microsoft® Windows XP SP2/3 / Vista SP1 (32 bit) / Windows 7 (32 bit, 64 bit).

Installation procedure

O Notice!

If present, uninstall Matlab Runtime before beginning with the installation of the LXSsoft Suite.

The LXSsoft Suite Setup.exe installation program is located on the supplied CD.

O Notice!

Copy this file from the CD to an appropriate folder on your hard drive.

Administrator privileges are required for the next steps.

- ♥ To start the installation process, double-click on file LXSsoft Suite Setup.exe.
- ♦ In the first window, click on Next.

In the next window, you can select whether you would like to install **LESsoft** only, or **LPSsoft** and **LRSsoft** in addition.

You will need **LPSsoft** and **LRSsoft** in addition for configuring light section sensors of the LPS or LRS series with your PC.

♦ Select the desired options and click on Next and, in the next window, click on Install.



The installation routine starts. After a few seconds, the window for selecting the installation language for the Matlab Compiler Runtime (MCR) appears. The MCR is used for 3D visualization. It is only available in English or Japanese.


Therefore keep in the Choose Setup Language window the selection English and click on OK.




Depending on the configuration of your Windows system the adjacent dialog can also appear (missing component VCREDIST X86).

♥ Click on Install

Two additional installation windows will appear, which do not require any further entry.

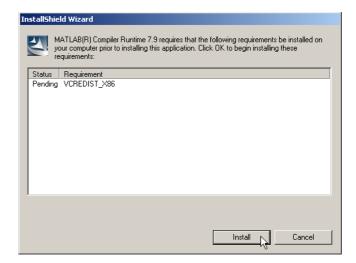

After some time (up to several minutes depending on the system configuration) the start screen of the MCR installer will appear. \$\\$ Click on Next.

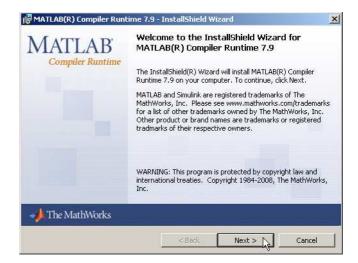


The window for entering user data appears.

Enter your name and the company name and then click on Next.

It is essential that you retain the default folder in the window for the selection of the installation path (Destination Folder).

The standard path is

C:\Programs\MATLAB\MATLAB Compiler Runtime\.

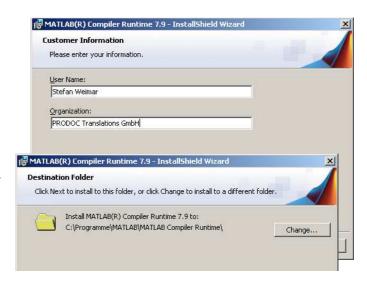


LES 36 Hl... - 02 2014/06

Light section sensor for object measurement

The installation will start and the adjacent status window will be displayed. This can again take several minutes.

Following successful MCR installation, the InstallShield Wizard Completed window appears.

Click on Finish to end the MCR-installation.

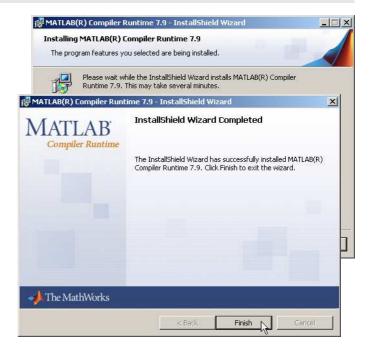

The window for selecting the installation path for **LESsoft** now appears.

♦ Keep the default folder and click on Next.


The installation of **LESsoft** starts. If you also selected **LPSsoft** and **LRSsoft** for installation, upon completion of the **LESsoft** installation, the same window then reappears for entering the installation path for **LPSsoft** and **LRSsoft**.



Upon completion of the installation process, the adjacent window appears.

The installation routine added a new Leuze electronic program group in your start menu that contains the installed programs LESsoft and, if selected, LPSsoft and LRSsoft.

Click on Finish and then start the desired program from the Start menu.

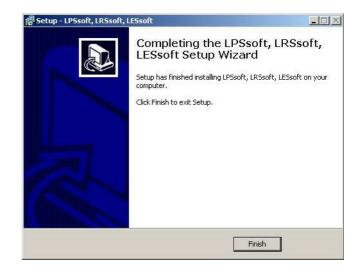

Possible error message

Depending on the system configuration the adjacent error message can appear at this point.

The cause of this error message is a bug in the MCR installation routine, which does not set the environment variable Path correctly in some systems.



That, however, can easily be corrected without reinstallation of the MCR.

- Open the System properties window located in the System control of Windows under System.
- \$ Go to the Advanced tab and click on Environment variables.

The Environment variables window opens.


- ♦ Scroll down in the System variables area until you find the Path entry.
- ♦ Click on Path and then on Edit

The Edit system variable window opens.

There in the Variable value field you will find the ; C:\Programs\MATLAB\MATLAB Compiler Runtime\v79\runtime\win32 entry right at the end.

- If this entry is missing, copy the entry from this document and insert it together with the preceding semicolon.
- Then click on oκ and close also all further windows using oκ.
- Shut Windows down, restart Windows and then start **LESsoft** by double-clicking on it.

Now the start screen of **LESsoft** appears, as described in chapter 8 of the LES technical description.

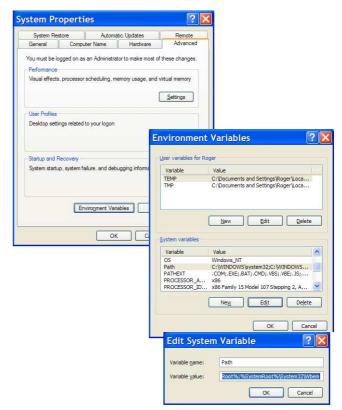

LES 36 Hl... - 02 2014/06